

Calcified lesions


Prevalence of calcified coronary lesions

Moderate-severe calcification in 13 DES studies


RAVEL	23.3% (27/116)
SIRIUS	17.1% (91/531)
E-SIRIUS	16.1% (28/174)
C-SIRIUS	12.0% (6/50)
TAXUS IV	18.3% (121/660)
TAXUS V	32.5% (185/570)
TAXUS VI	29.7% (65/219)
ENDEAVOR II	23.7% (140/590)
ENDEAVOR III	17.9% (78/436)
ENDEAVOR IV	33.2% (513/1546)
SPIRIT II	31.4% (91/290)
SPIRIT III	27.8% (277/997)
COMPARE	38.5% (693/1799)
Total	29.0% (2,315/7,978)

ADAPT-DES (11 center all-comers registry): Mod-Sev Calcification


N = 8,582 pts

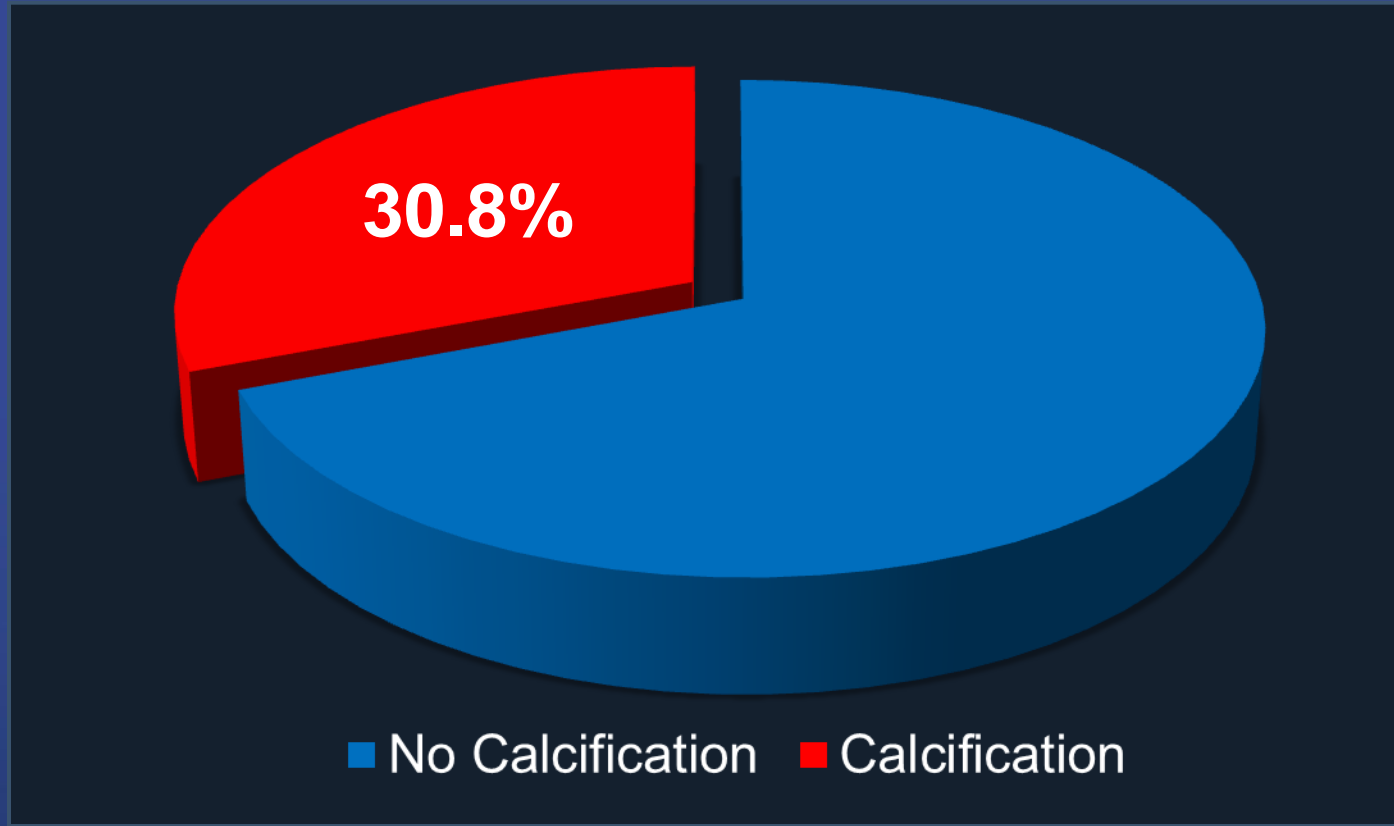


Frequency of Mod-Sev Calcification in NSTEMI-ACS and STEMI PCI population: (ACUITY and HORIZONS-AMI)

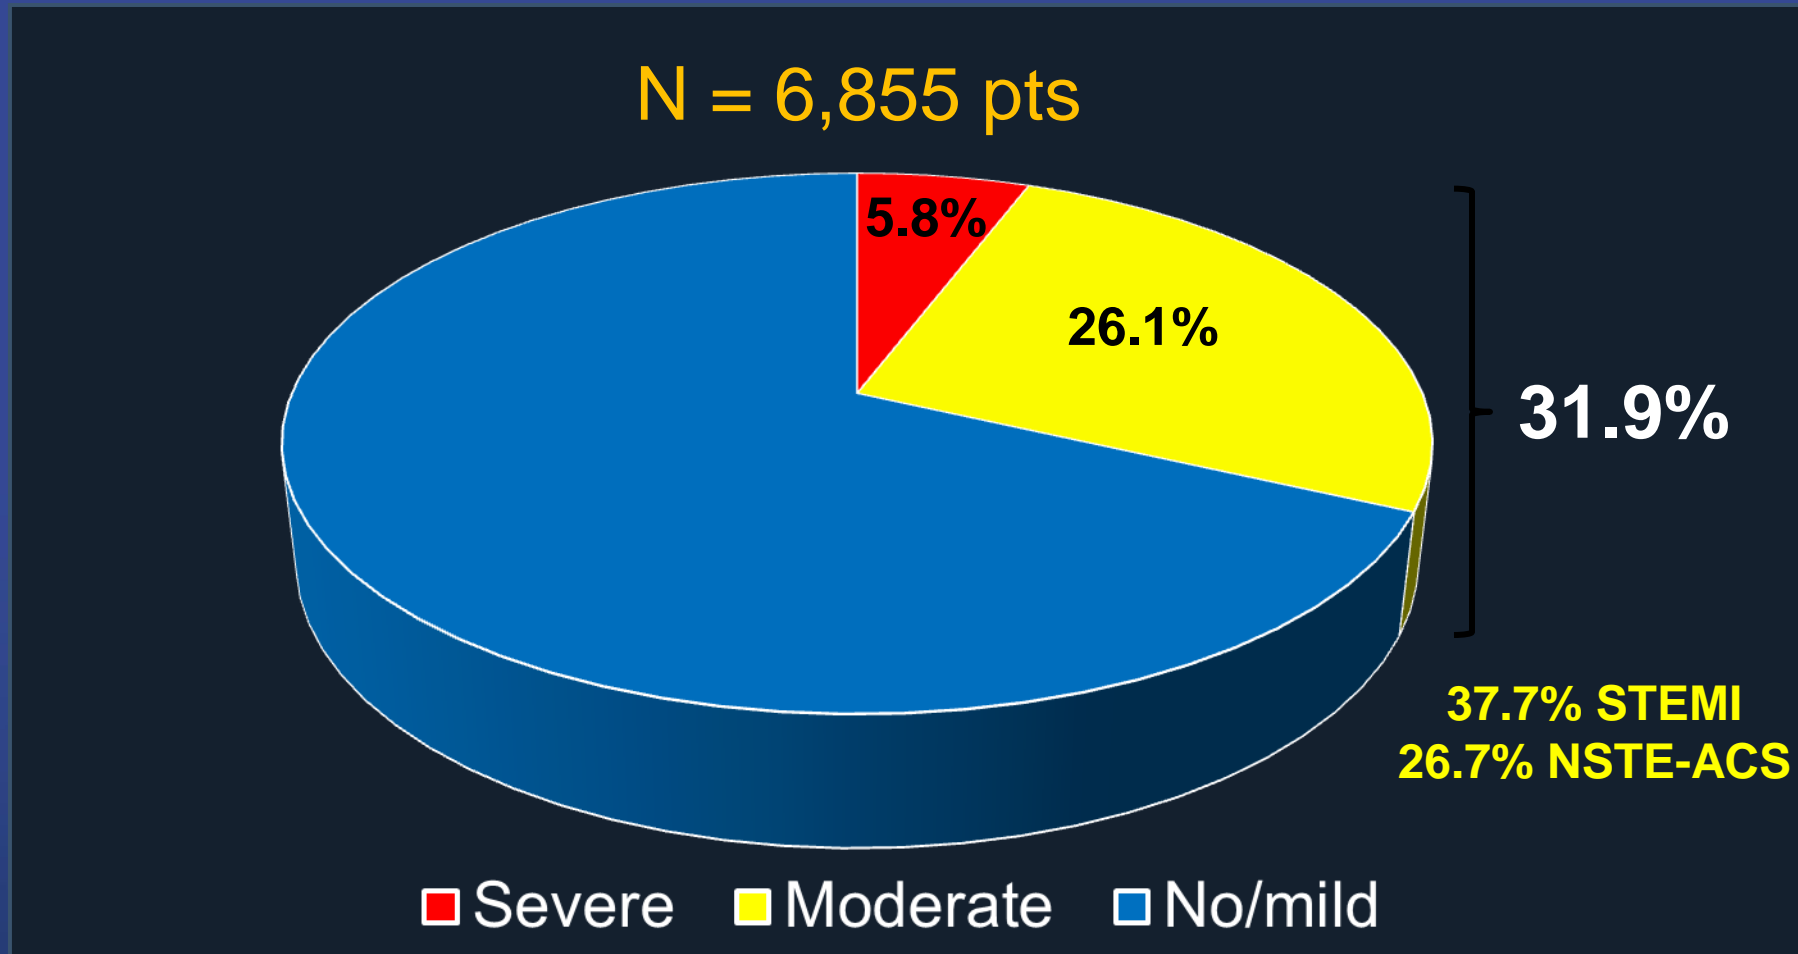

Frequency of “heavy” calcification in the SYNTAX trial: Randomized + Registry N=2,636 pts with LM or 3VD

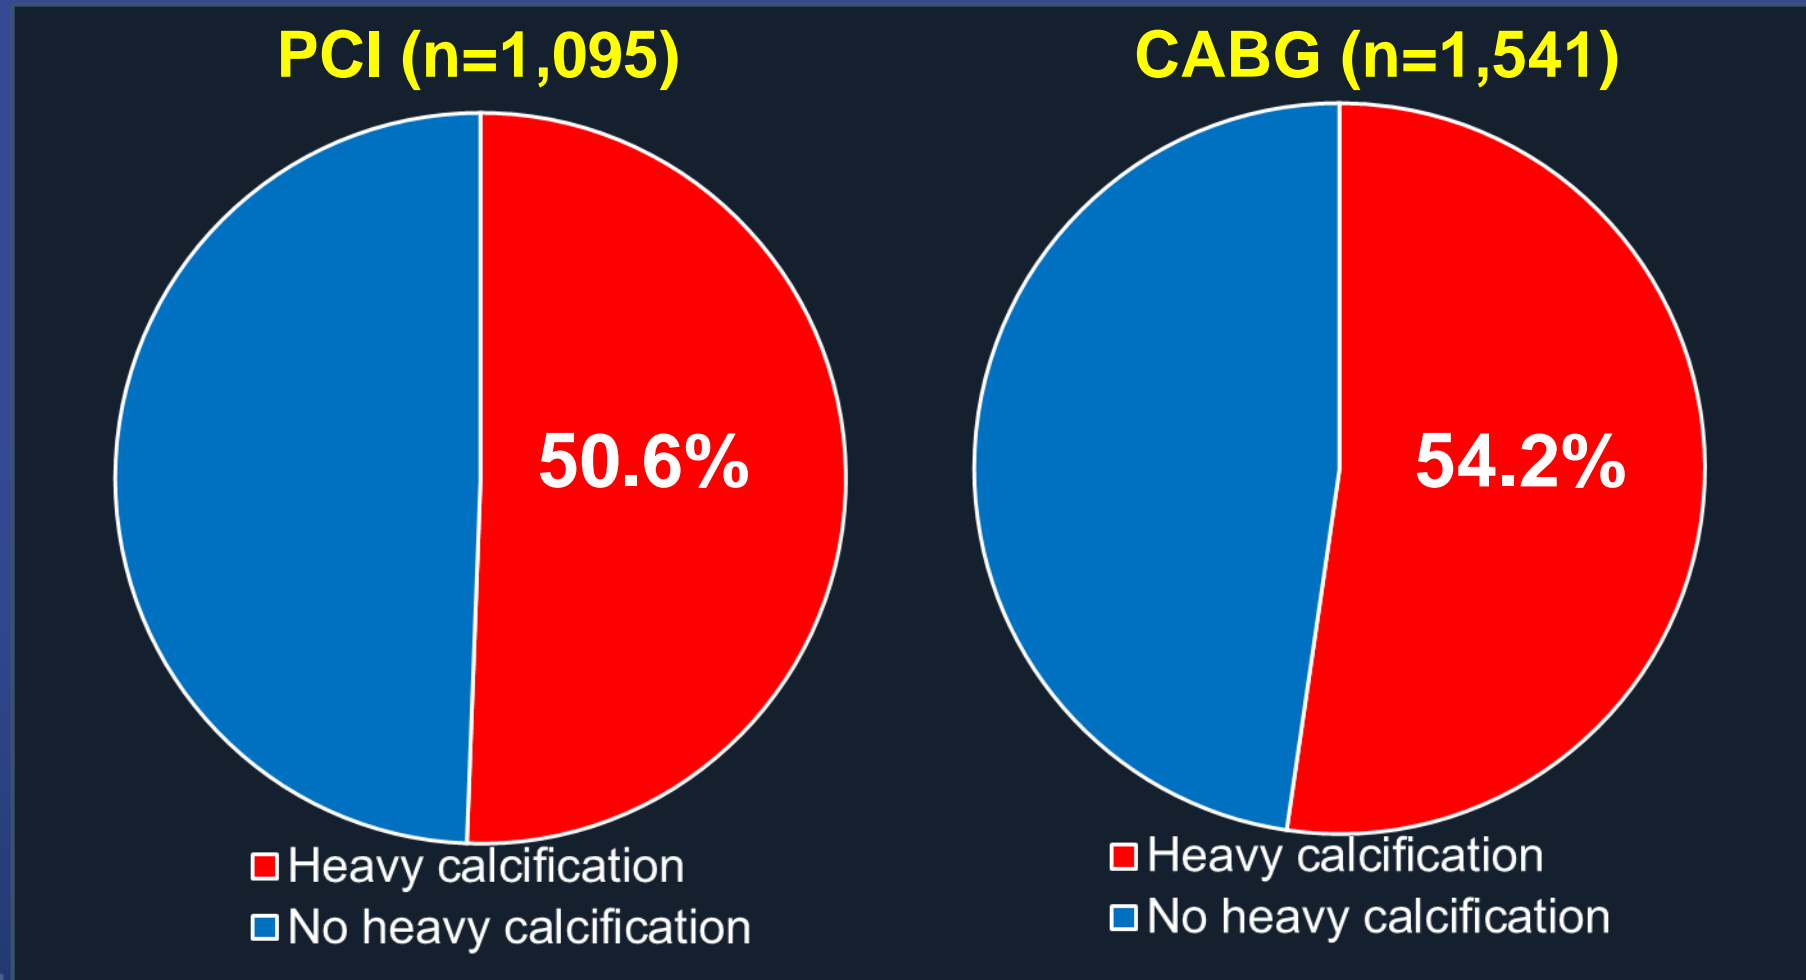


Stent Expansion in Calcified Lesions

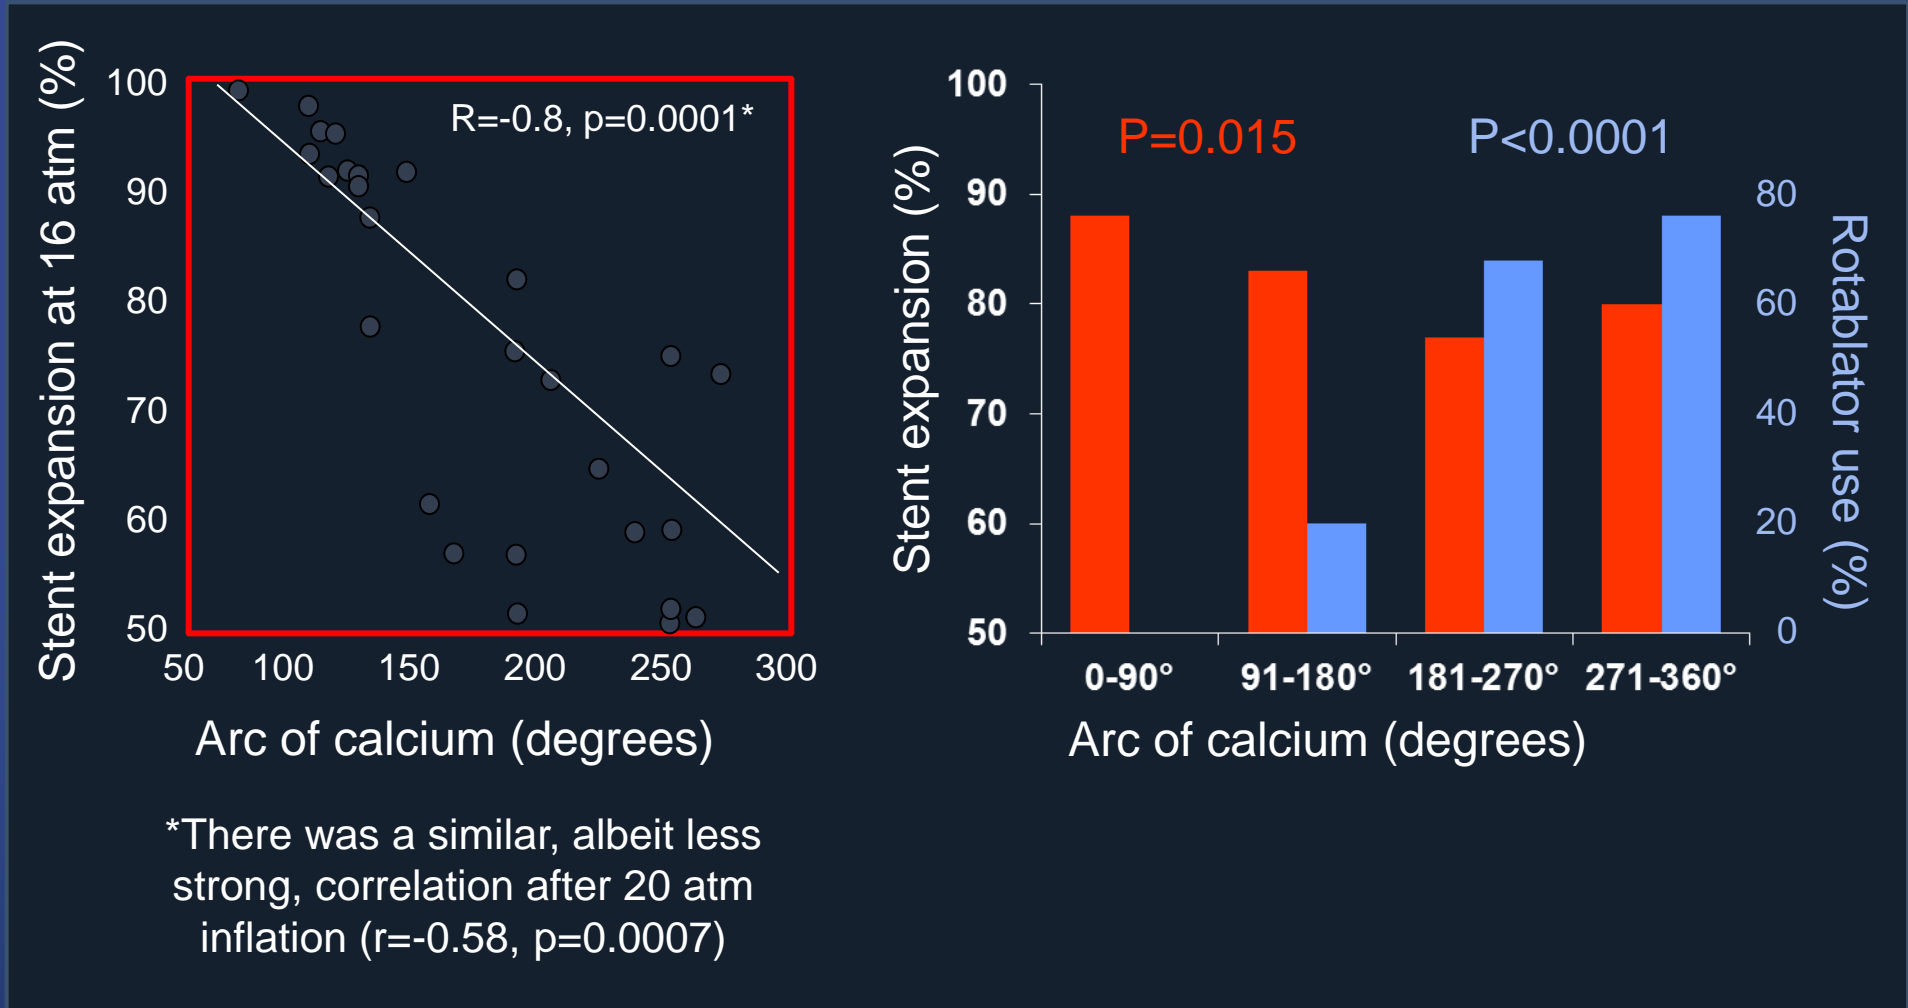

ADAPT-DES (N=8,582)

Target vessel failure at 2 years

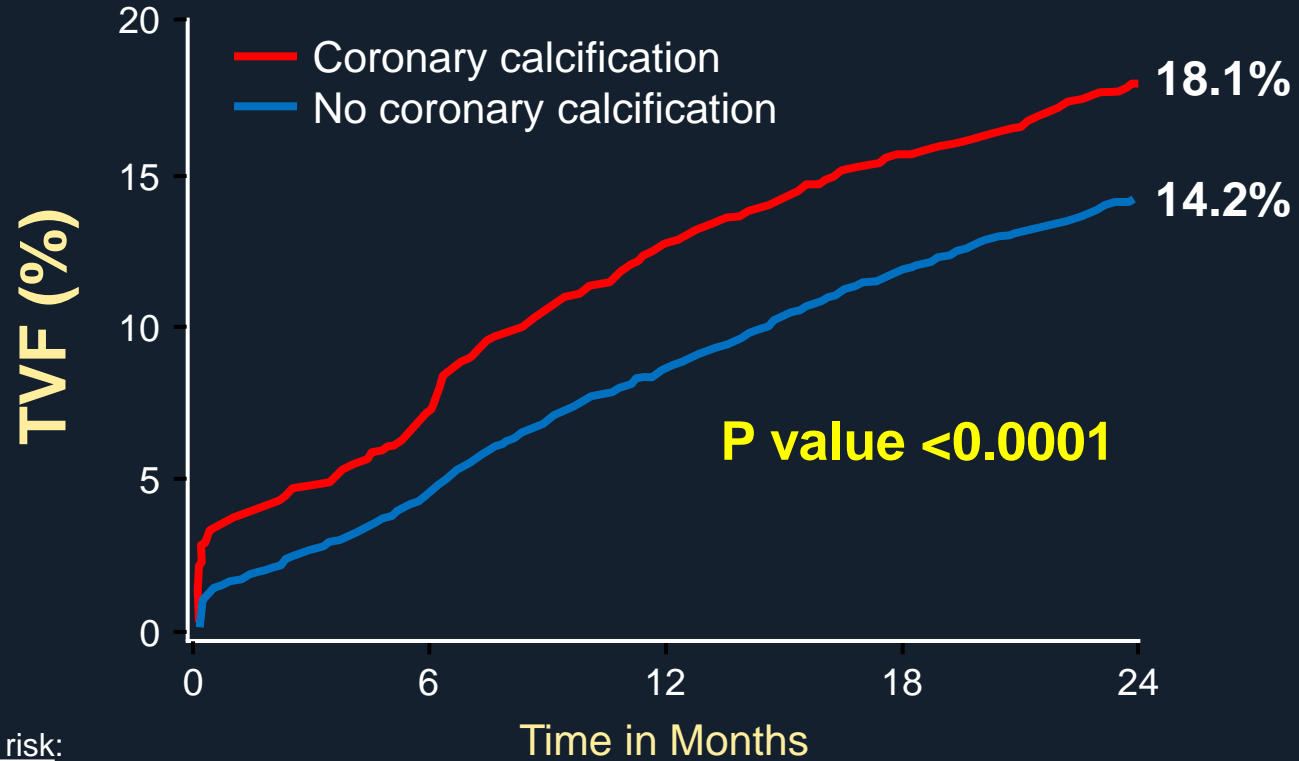

No at risk:


CCA	2,644	2,426	2,277	2,178	1,198
No CCA	5,938	5,505	5,177	4,849	2,392

ADAPT-DES (N=8,582): Calcification and 2-year Events

	Calcification		Unadjusted <i>p</i>	Adjusted HR [95% CI]	Adjusted <i>p</i>
	No (n=5,938)	Yes (n=2,644)			
TVF	14.2%	18.1%	<0.0001	1.23 [1.09, 1.39]	0.0008
MACE	5.6%	8.3%	<0.0001	1.47 [1.22, 1.76]	<0.0001
Death	3.5%	4.8%	0.003	1.15 [0.90, 1.46]	0.26
CV death	2.3%	2.8%	0.09	1.09 [0.80, 1.48]	0.60
MI	4.0%	6.4%	<0.0001	1.61 [1.30, 1.99]	<0.0001
Clinically- driven TVR	9.5%	10.4%	0.16	1.10 [0.94, 1.29]	0.24
Stent thrombosis	0.9%	1.1%	0.32	1.49 [0.92, 2.43]	0.11

Stent Expansion Indexes to Predict Clinical Outcomes: An IVUS Substudy From ADAPT-DES


CENTRAL ILLUSTRATION: 2-Year Rate of Clinically Driven Target Lesion Revascularization or Definite Stent Thrombosis Stratified by Minimum Stent Area Quartiles and Minimum Stent Area/Vessel ($\leq 38.9\%$ Versus $> 38.9\%$)

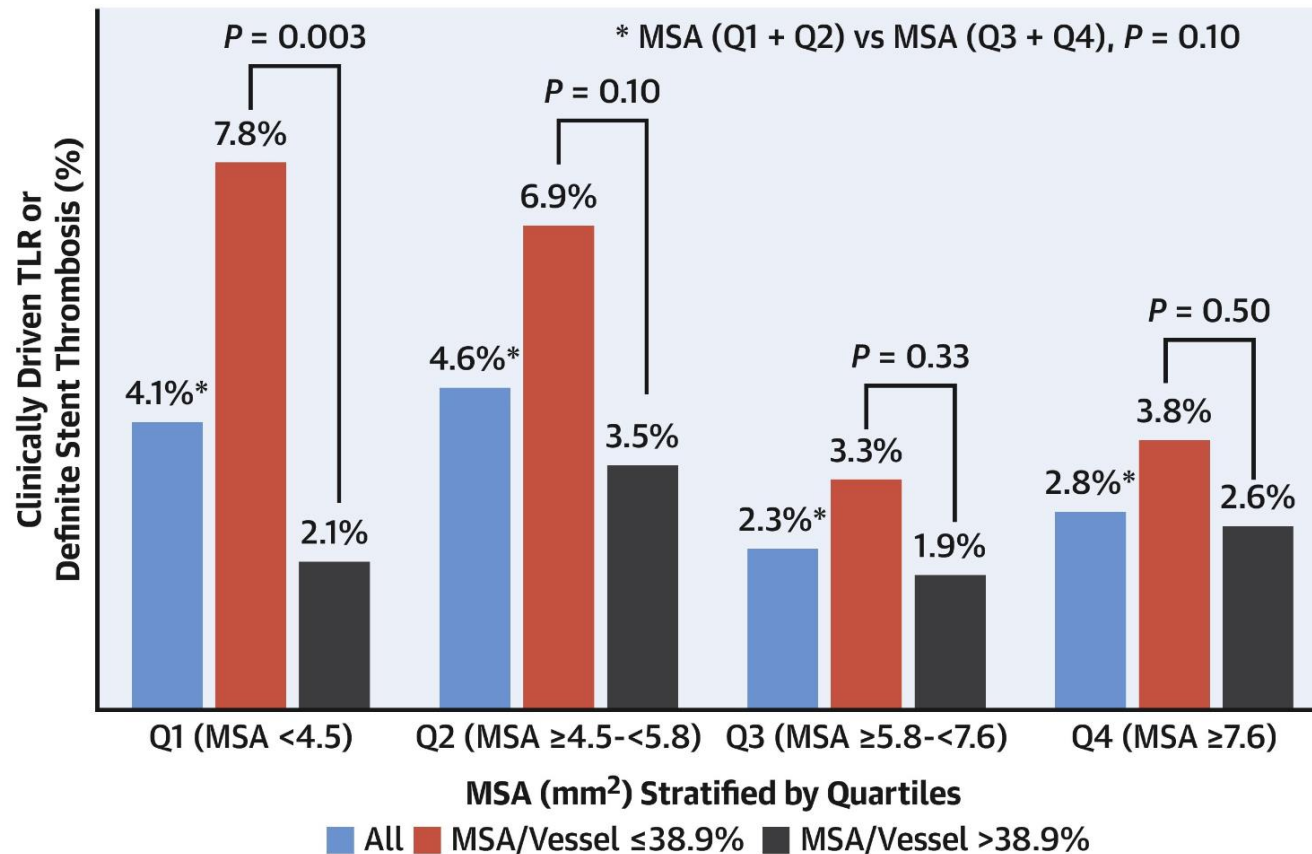

Stent/vessel area at the MSA site, an index of relative stent expansion, was **superior** to absolute MSA and other expansion indexes in predicting 2-year clinically driven **TLR** or **definite stent thrombosis**


Data from IRIS-DES Registries

17,084 patients who underwent PCI with DES

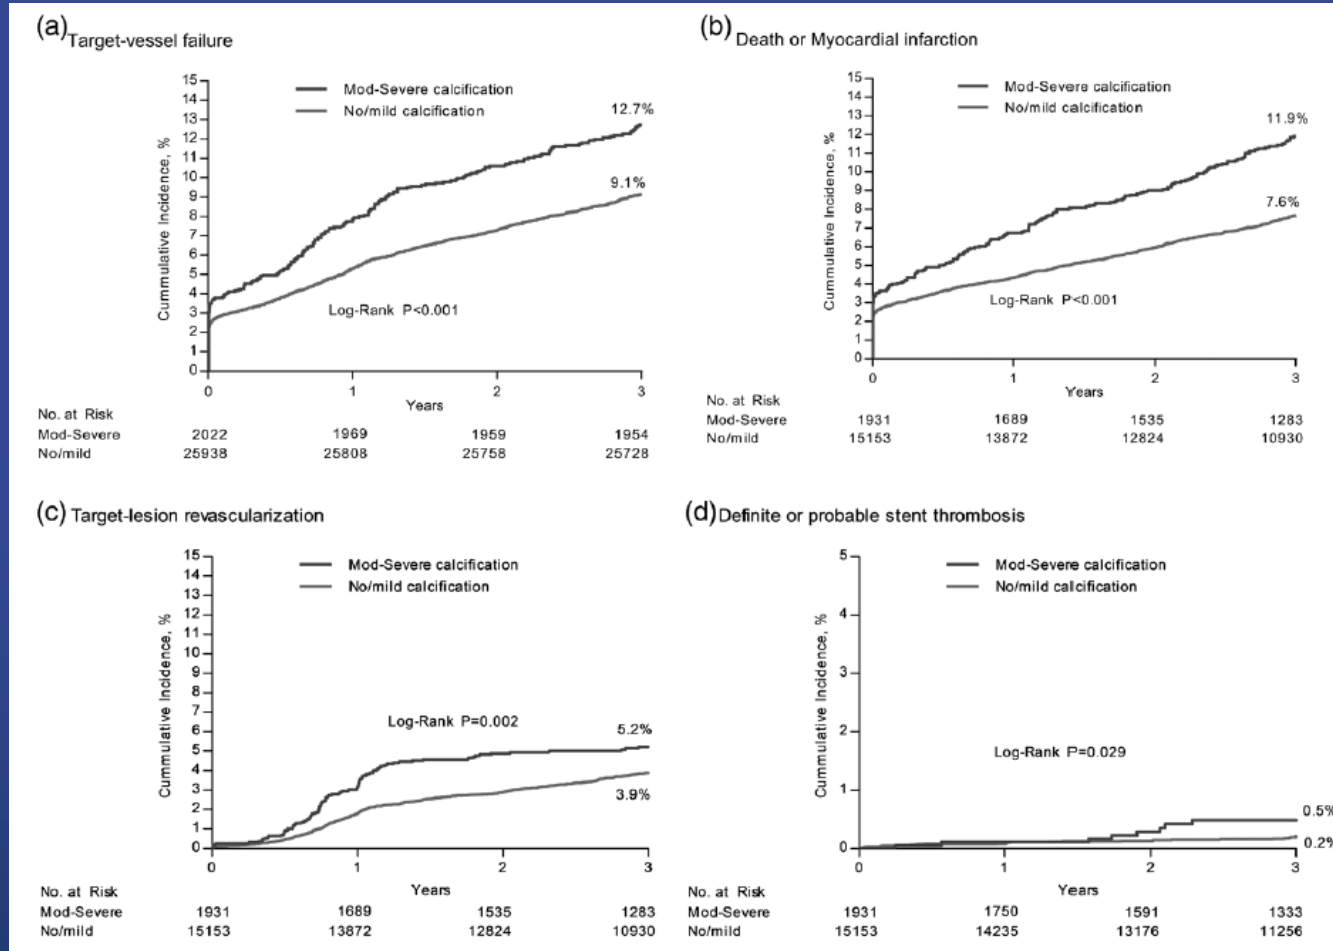

TWENTE and DUTCH PEERS (TWENTE II): Impact of Severe Calcification with 2nd Generation DES

1,423 pts with stable angina; 342 (24%) with severe calcification

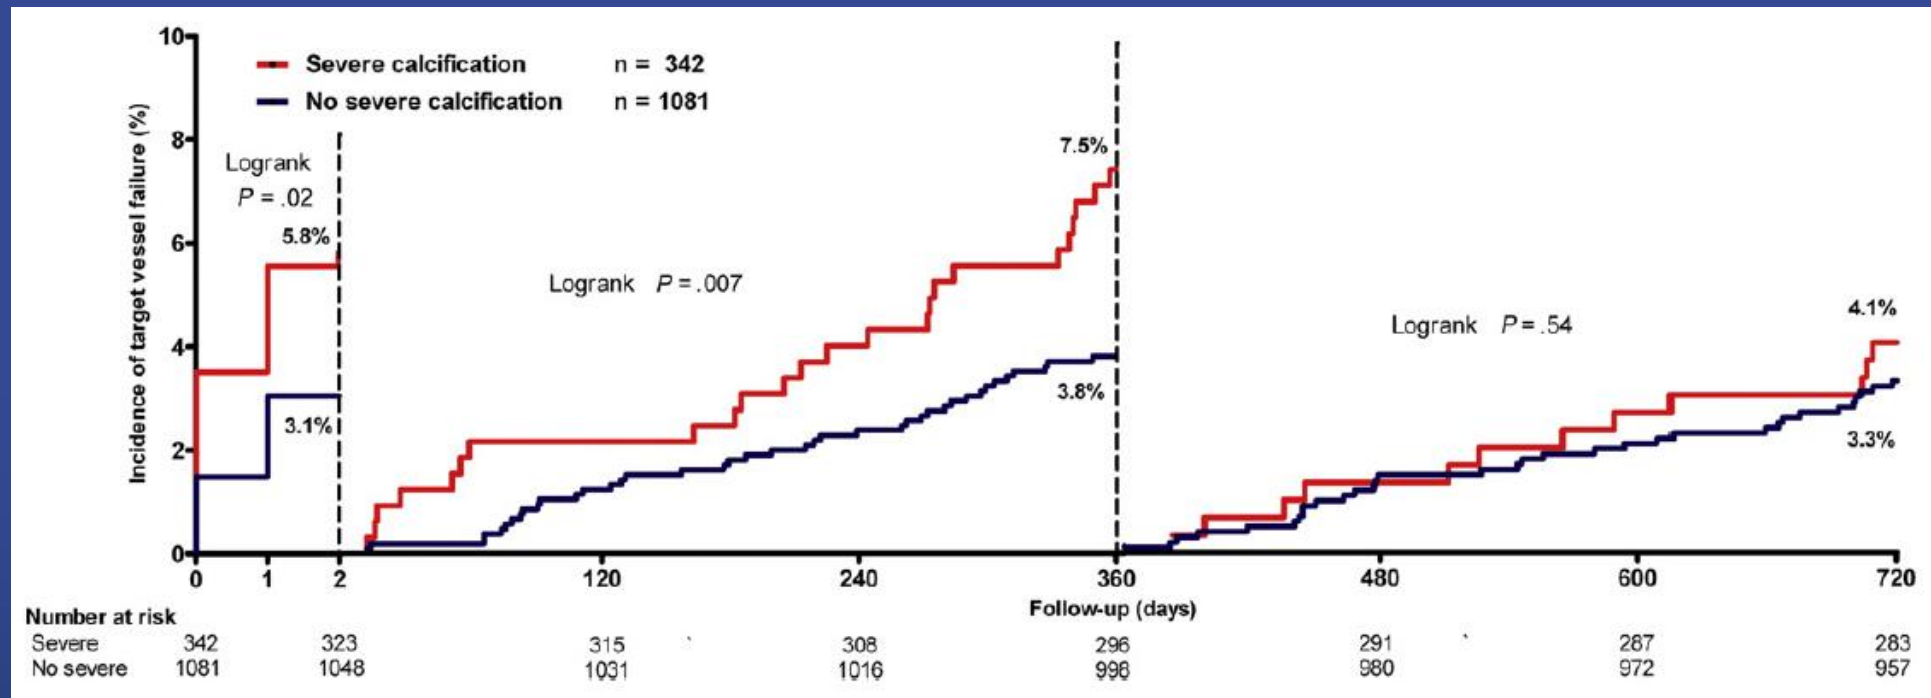


At 2 years, TVF was 16.4% vs. 9.8%, $p=0.001$
predominantly driven by events in the first 48 hours and up to 1 year

Of note, 2 year definite ST was 1.8% vs. 0.4%, $p=0.02$

ACUITY/HORIZONS-AMI: Implications of Calcified Lesions on PCI in ACS

Post-PCI	Moderate/Severe (n=2,958)	None/Mild (n=5,783)	P value
TIMI flow 0/1	2.6%	1.6%	0.001
TIMI flow 2	6.8%	5.2%	0.004
TIMI flow 3	90.6%	93.1%	<0.0001
No reflow	0.4%	0.1%	0.02
Perforation	0.1%	0.1%	0.41
Spasm	1.1%	0.6%	0.02
Dissection	2.9%	1.2%	<0.0001
Abrupt closure	0.5%	0.1%	0.001

ACUITY/HORIZONS-AMI: Implications of Calcified Lesions on PCI in ACS

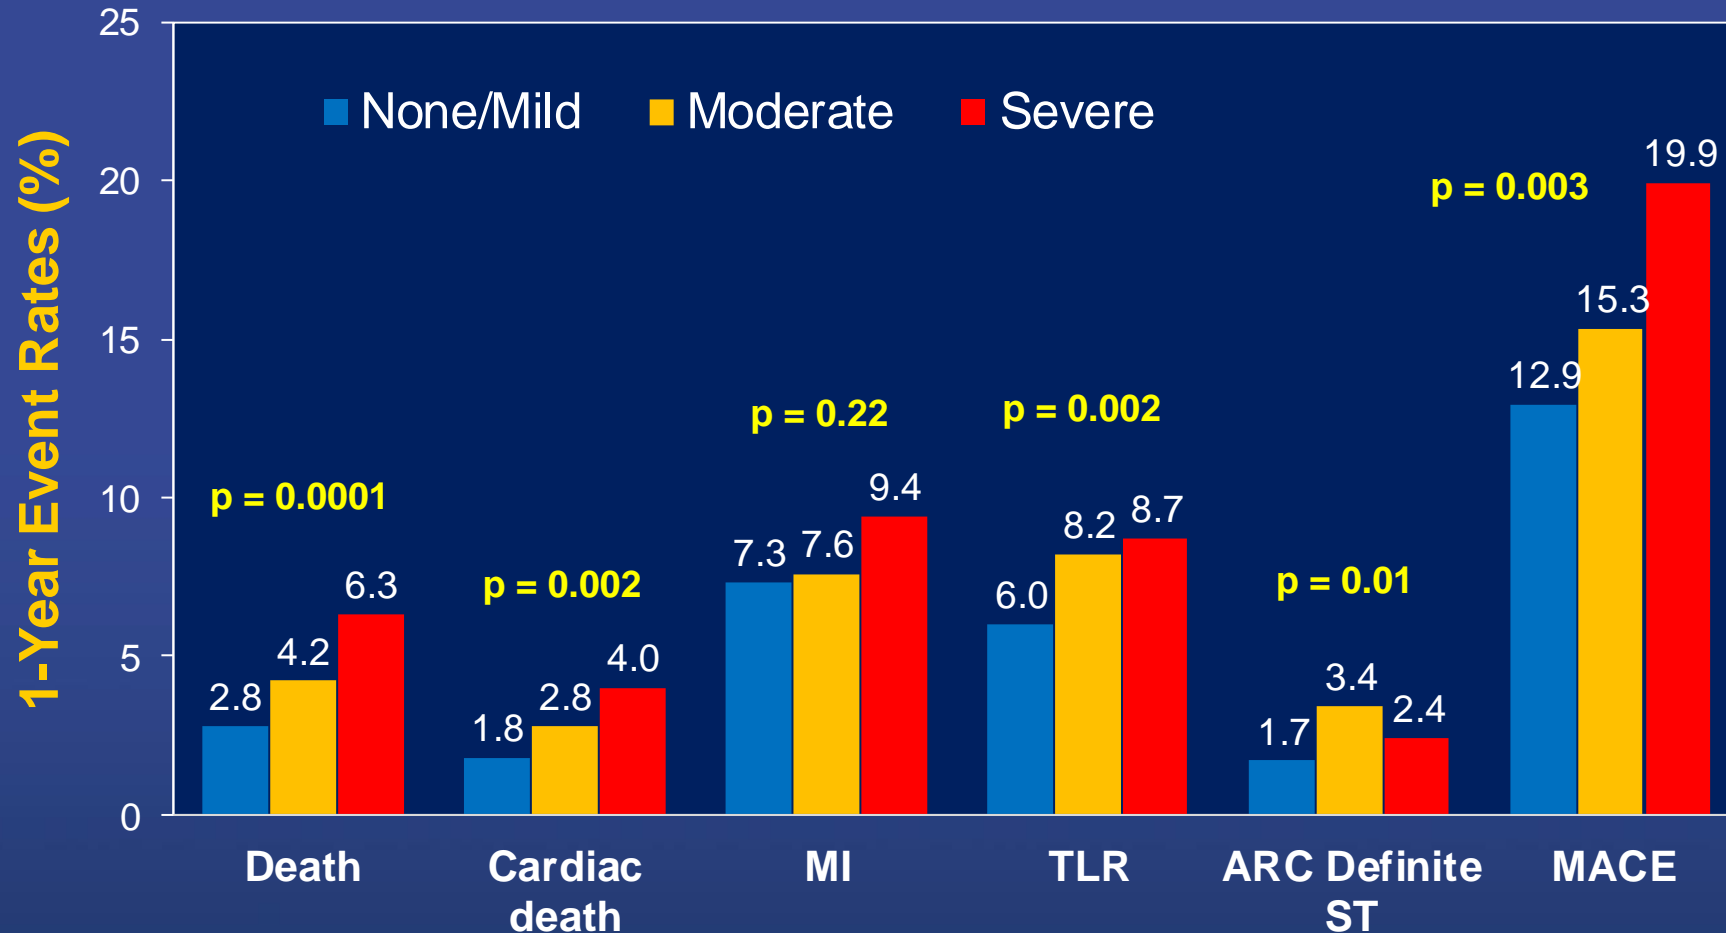


Généreux P et al. J Am Coll Cardiol 2014 13;63:1845-54

ACUITY/HORIZONS-AMI: Implications of Calcified Lesions on PCI in ACS


	Adjusted Hazard Ratio [95% CI]	P Value
Death	1.10 [0.81,1.48]	0.55
MI	1.06 [0.86,1.30]	0.58
Ischemic TLR	1.44 [1.17,1.78]	0.0007
ARC definite ST	1.62 [1.14,2.30]	0.007

Impact of calcification on percutaneous coronary intervention:

MACE-Trial 1-year results

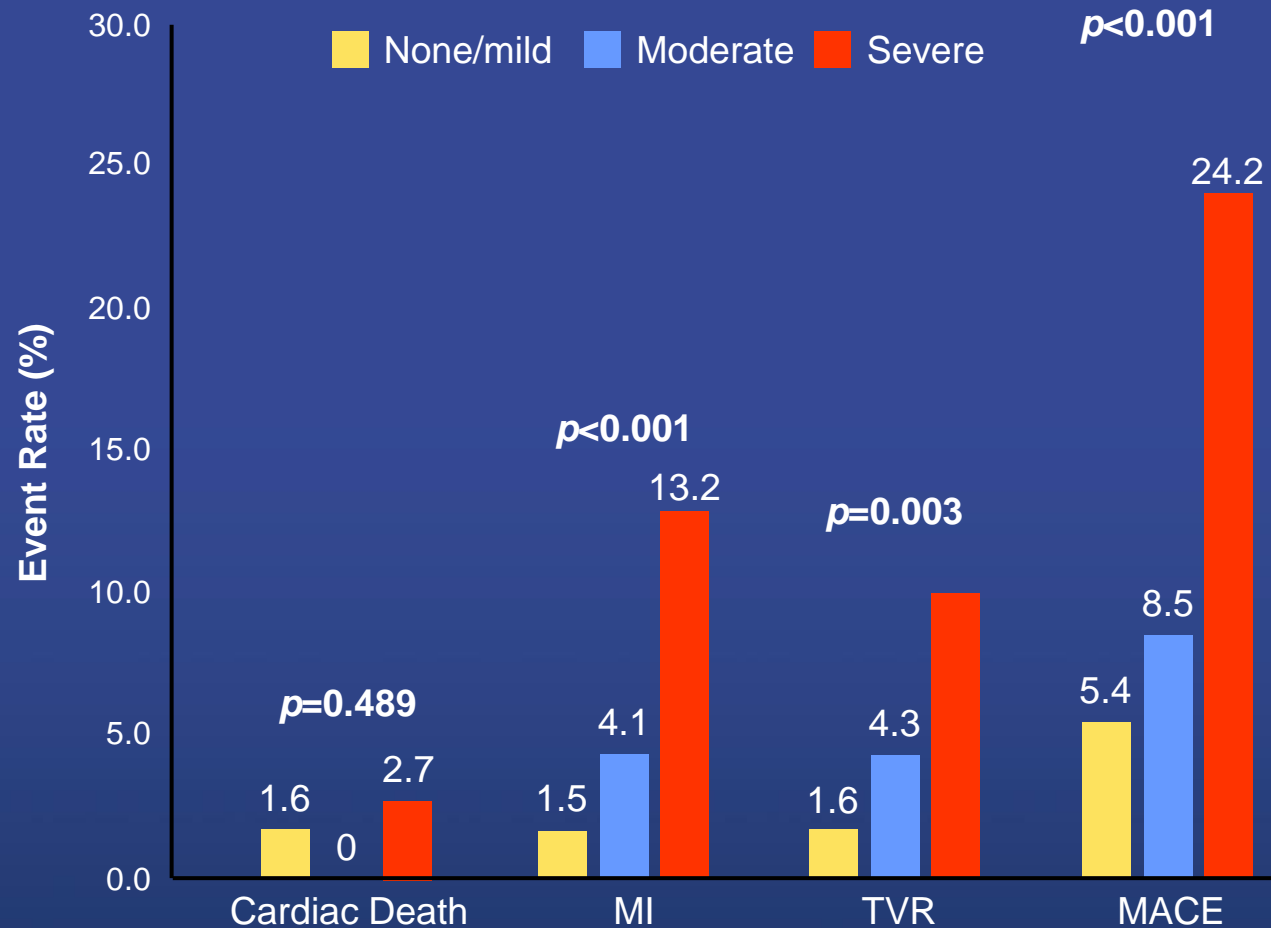


Coronary Calcification and Long-Term Outcomes According to Drug-Eluting Stent Generation

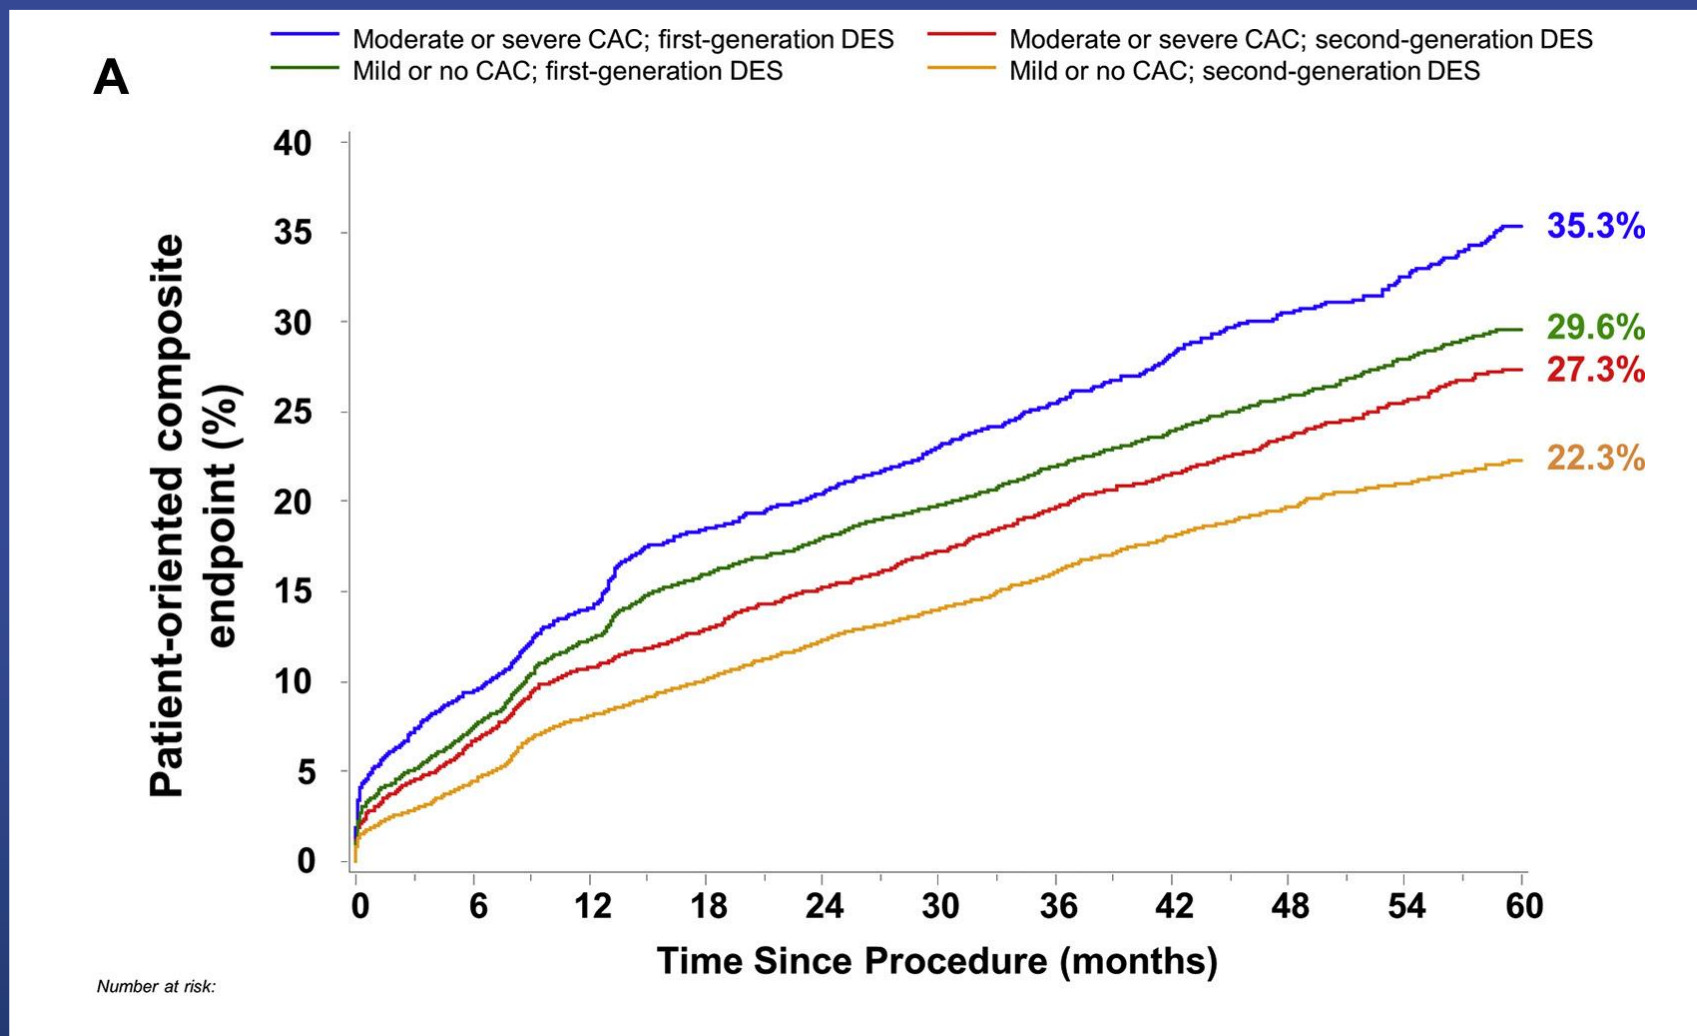

JACC Cardiovasc Interv. 2020 Jun 22;13(12): 1417-1428.

Coronary Calcification and Long-Term Outcomes According to Drug-Eluting Stent Generation

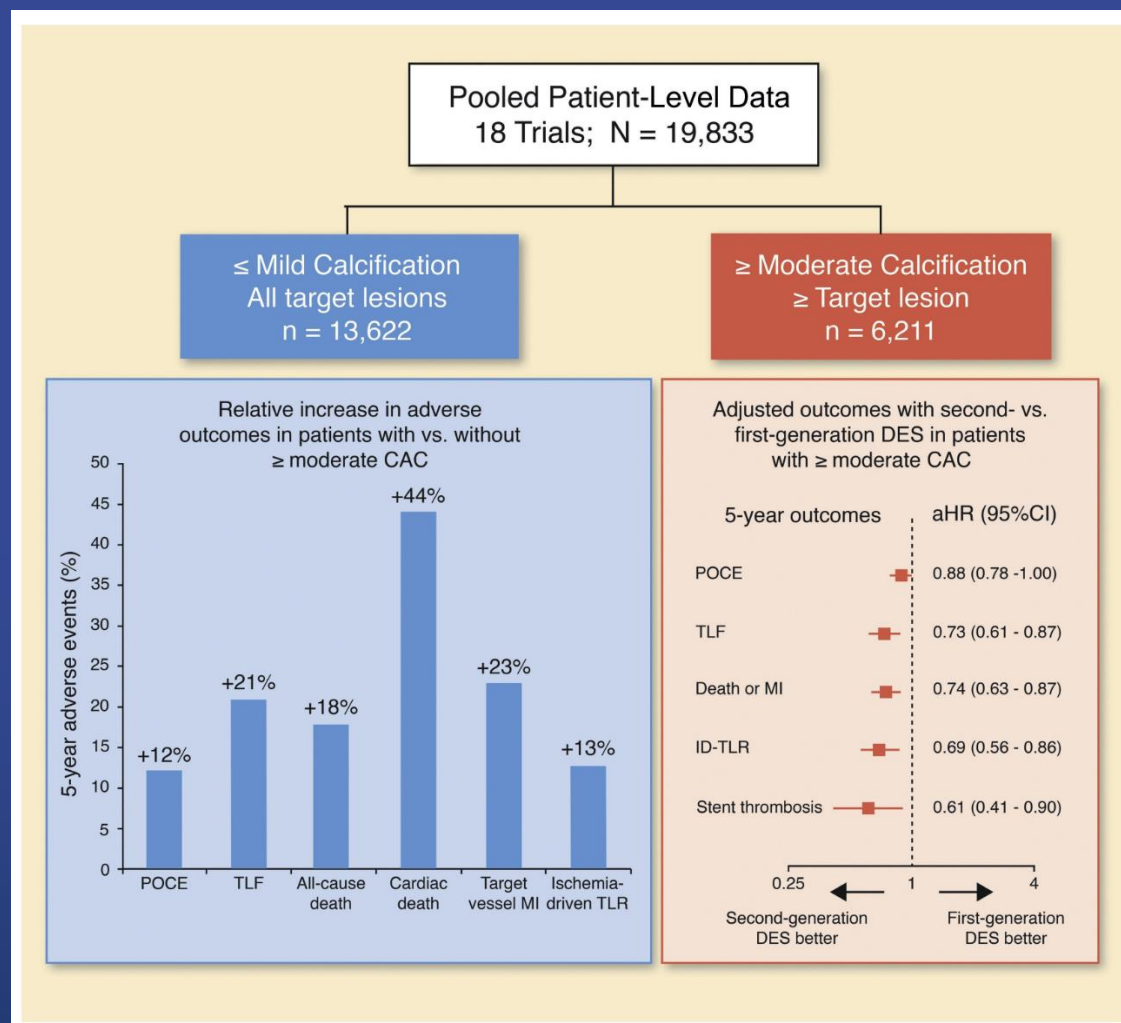


PCI of target lesion moderate or severe CAC was associated with adverse patient-oriented and device-oriented **adverse outcome** at 5 years

Treatment of Calcified Lesions


NC balloons




Cutting balloon

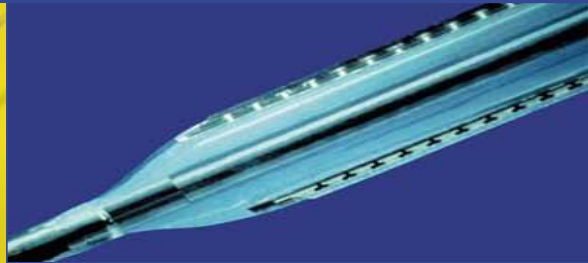


Chocolate PTCA balloon

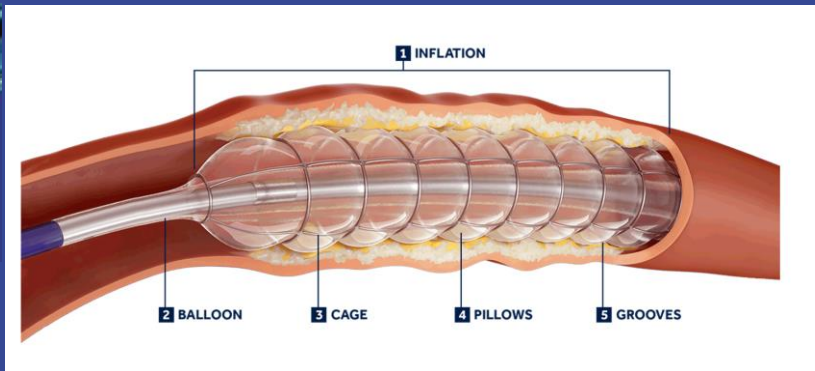


Laser

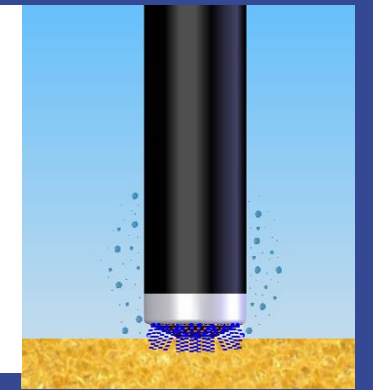


Angiosculpt

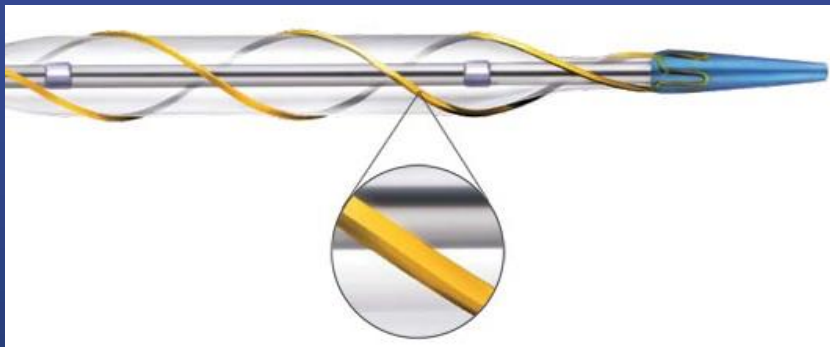

Rotational atherectomy

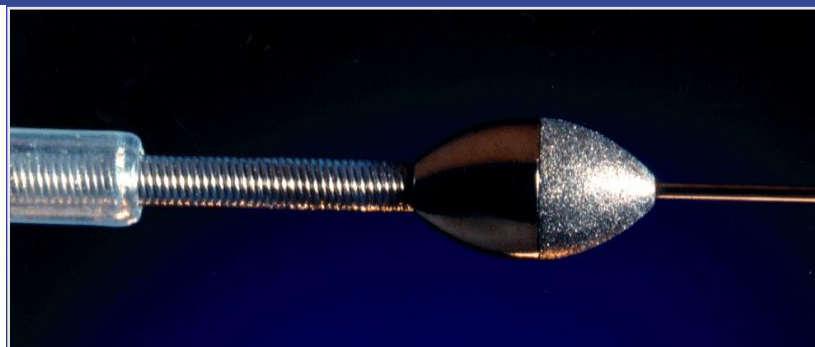

Orbital atherectomy

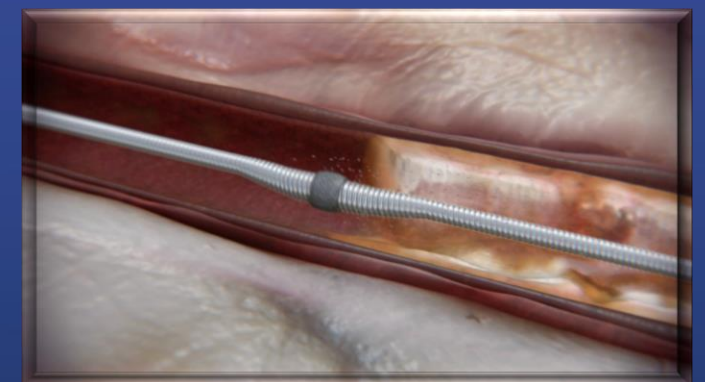

New Technics

Intravascular lithotripsy


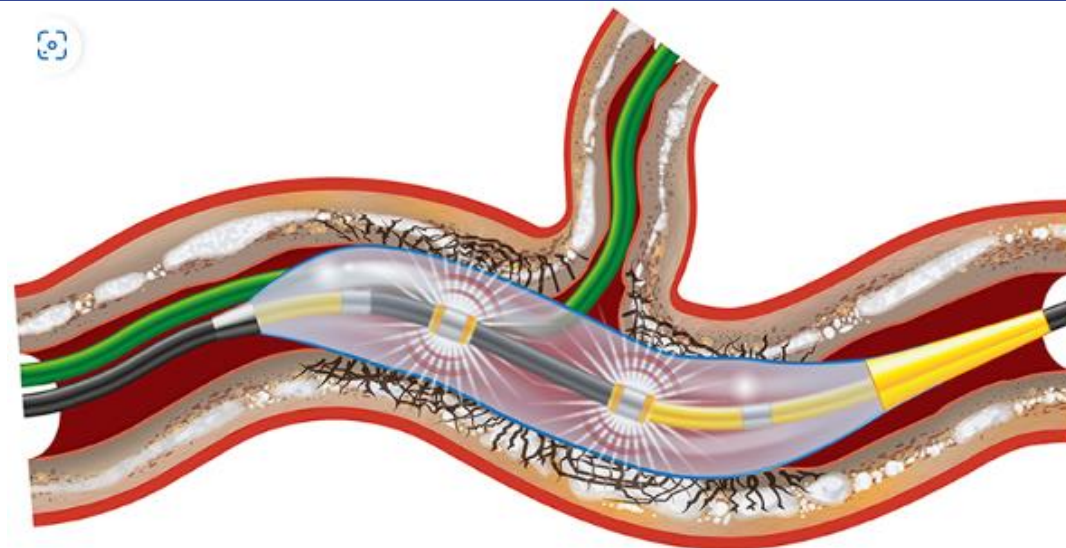


Photo Credit: Shockwave Medical

Calcium Fracture and Relation to Outcomes

61 pts with heavily calcified lesions studied serially with OCT
Fracture was seen in 48% (more frequently with CB or atherectomy)

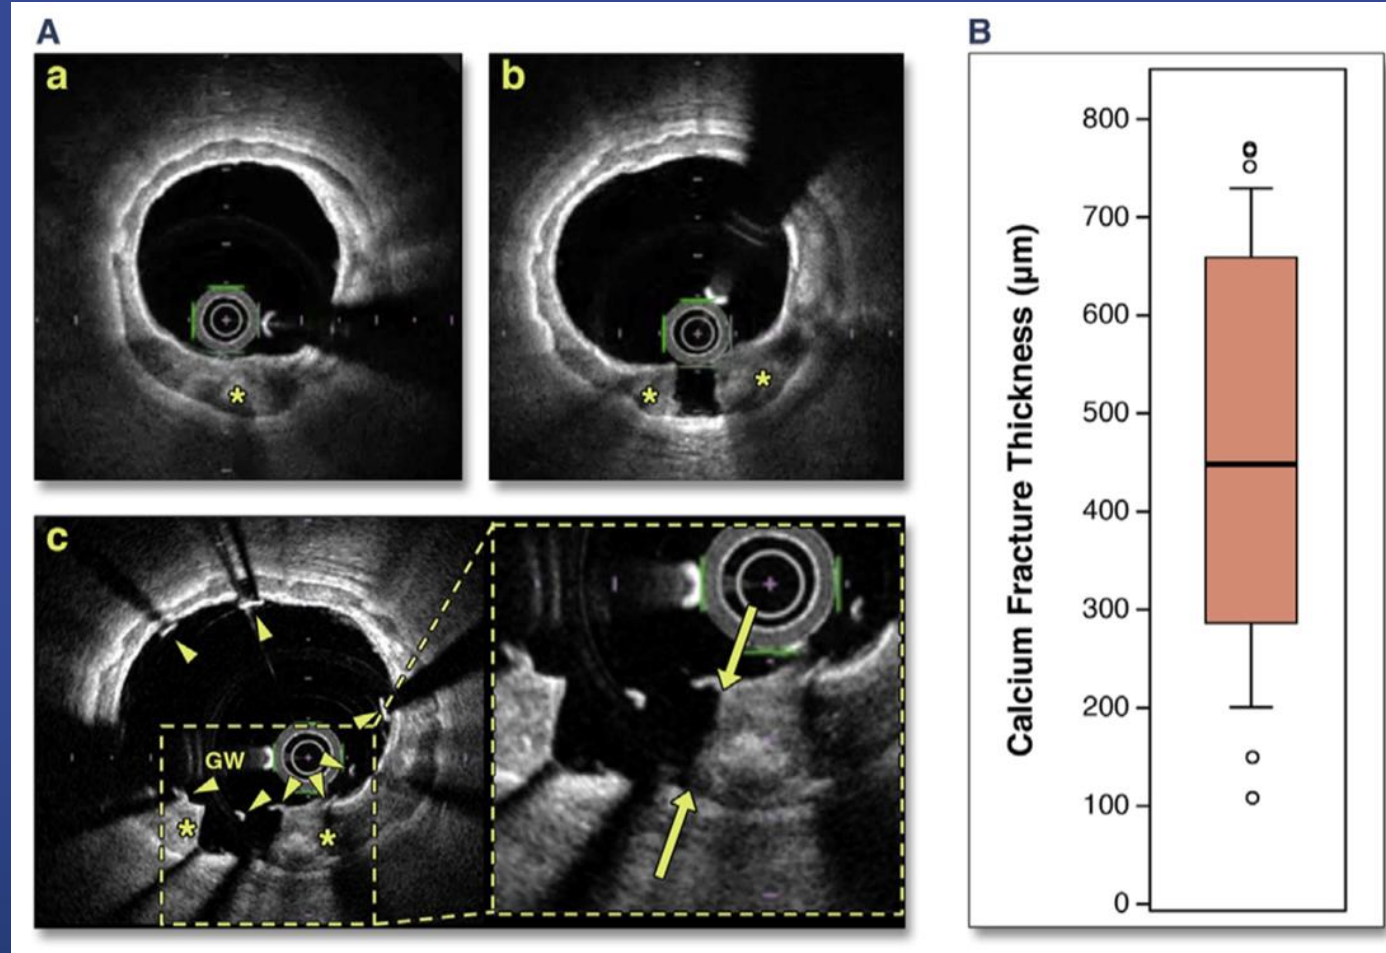

Fracture was associated with greater MSA and less restenosis/ID-TLR

Optical frequency-domain predictor good stent expansion after atherectomy


50 de novo heavily calcified lesions that underwent OFDI-guided RA)

Variable	Univariate predictors		Multivariate predictors		
	Standardized coefficient (β)	P	Standardized coefficient (β)	t-statistics	P
Diabetes mellitus	0.058	0.69			
Hemodialysis	-0.073	0.61			
Burr-to-artery ratio	0.009	0.95			
Arc of calcium	0.075	0.60			
Minimum thickness of calcium	-0.53	<0.001*	-0.45	-3.78	<0.001*
Maximum thickness of calcium	0.50	0.50			
Length of calcium	-0.10	0.90			
Dissection formation	0.43	0.002*	0.32	2.65	0.011*


Minimum of thickness of calcification in the intima and dissection formation were positively associated with good stent expansion after RA.

ADAPT-DES (11 center all-comers registry): Calcified lesion preparation

N = 2,644 patients

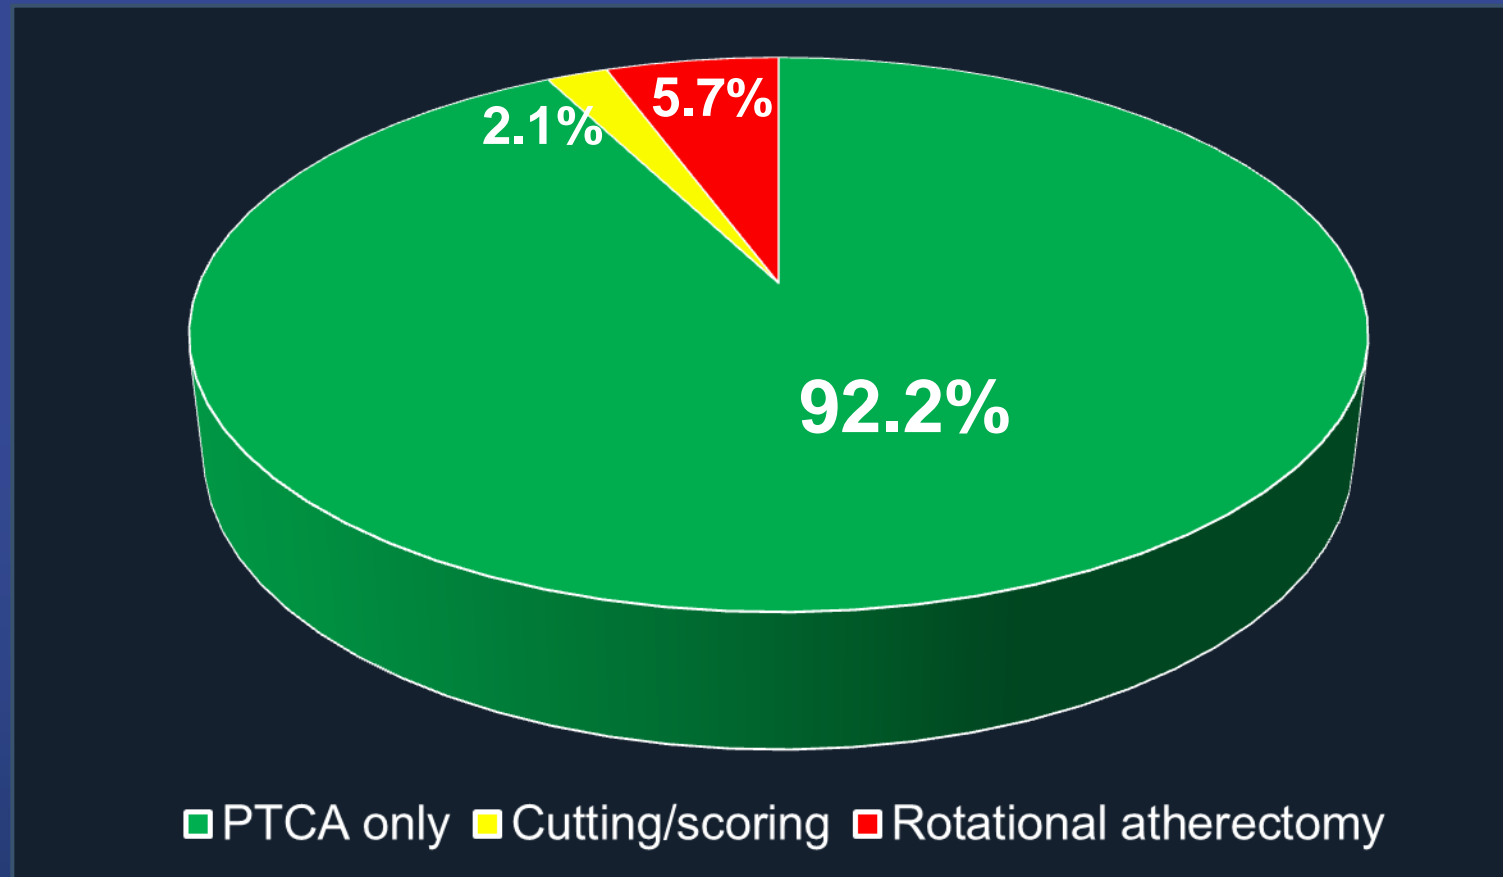


Potential Strategy for Calcified Lesions

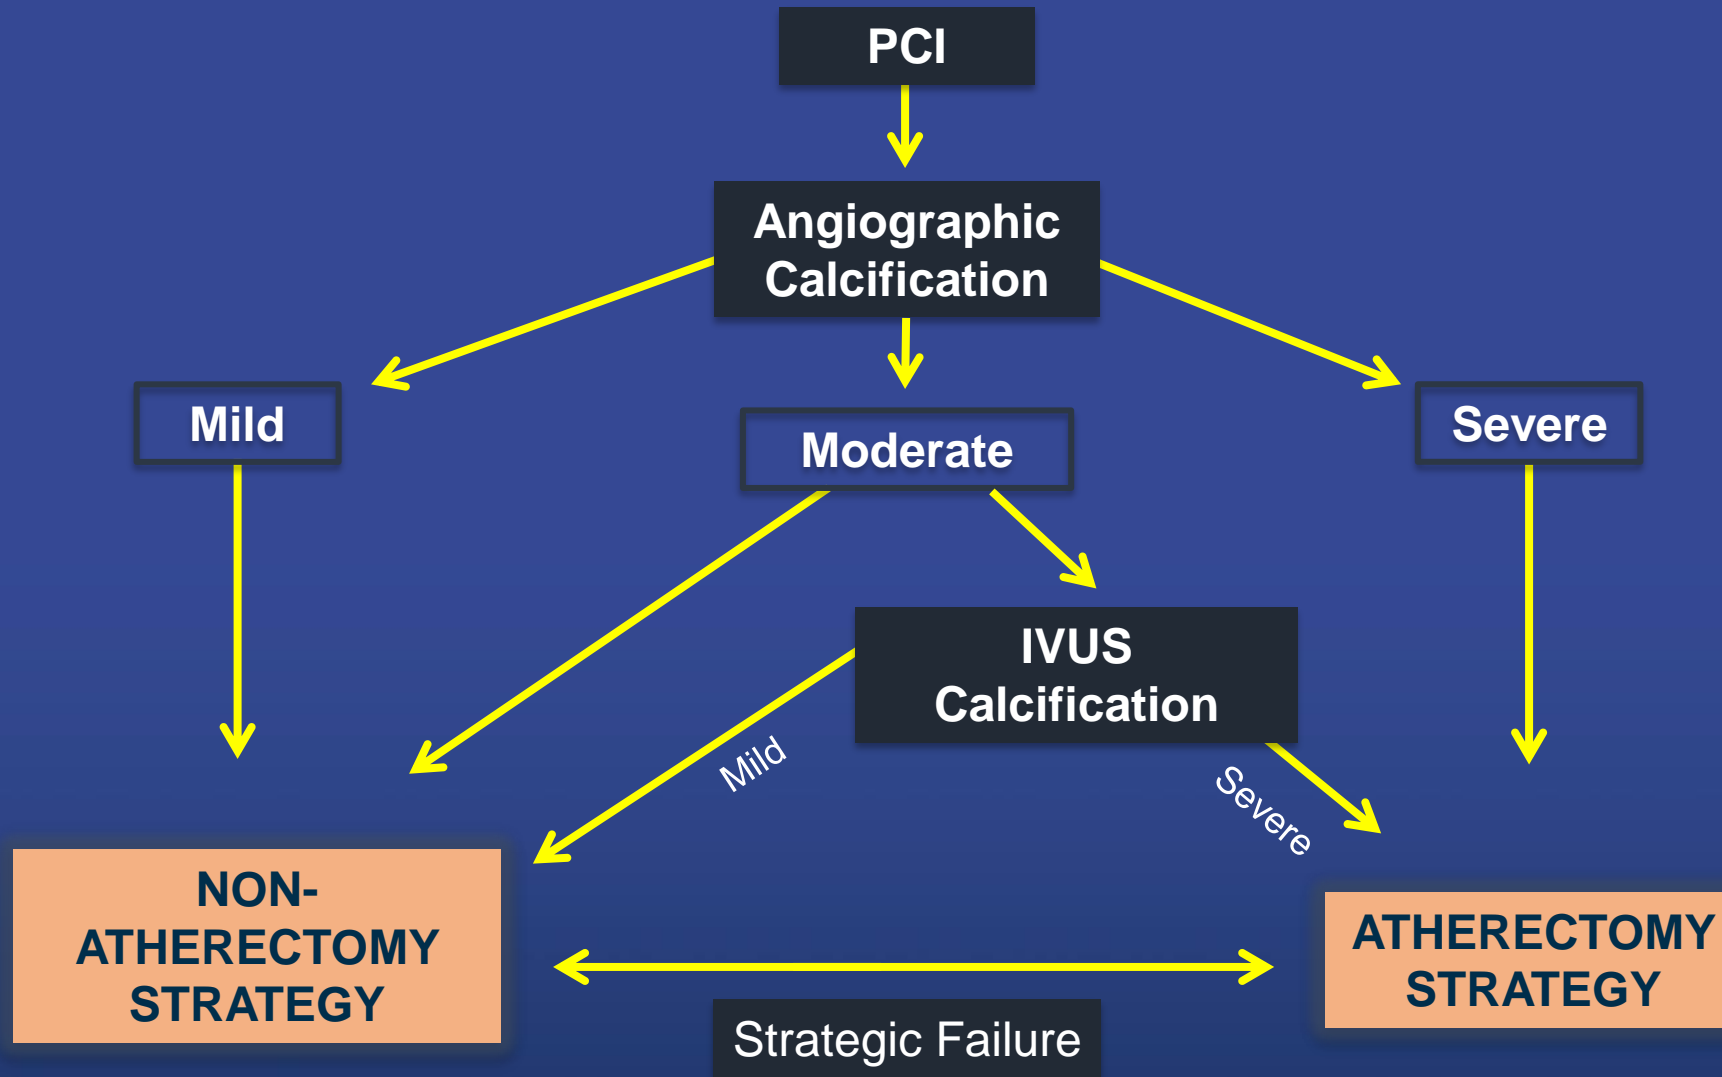

PCI Guideline recommendation

- In patients with fibrotic or heavily calcified lesions, plaque modification with **rotational atherectomy** can be useful to improve procedural success.
(class 2a-B)
- In patients with fibrotic or heavily calcified lesions, plaque modification with **orbital atherectomy, balloon atherotomy, laser angioplasty, or intracoronary lithotripsy** may be considered to improved procedural success.
(class 2b-B)
- **Cutting or scoring balloon angioplasty or rotational atherectomy** may be required in selected lesions—particularly those with heavy calcification—in order to adequately dilate lesions prior to stent implantation
- However, studies investigating the systematic use of these adjunctive technologies have **failed** to show clear clinical benefit.



Calcium Volume Index (CVI) Scoring System

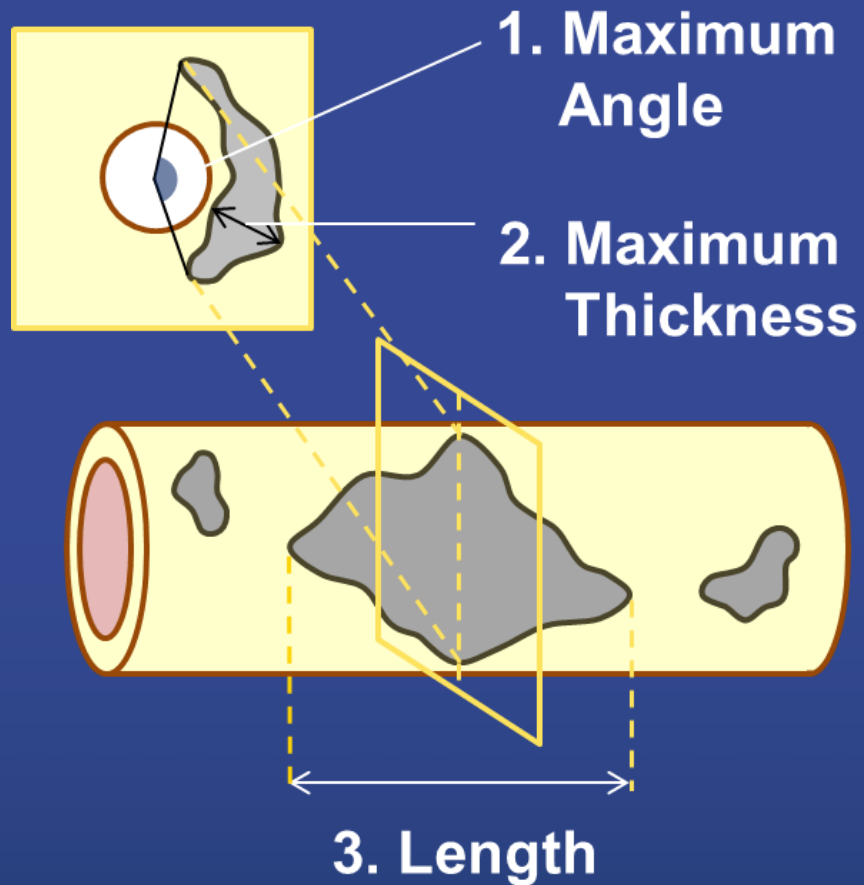

OCT-based CVI Score	
Angle	$\leq 180^\circ$ → 0 point
	$> 180^\circ$ → 2 points
Thickness	≤ 0.5 mm → 0 point
	> 0.5 mm → 1 point
Length	≤ 5.0 mm → 0 point
	> 5.0 mm → 1 point
Total score: 0 to 4 points	

IVUS-Based Calcium Scoring System

- Example:
Calcium Score=0
- Length of Ca $>270^\circ = 4.1\text{mm}$
 - Calcified nodule (-)
 - Vessel diameter = 4.4mm
 - Reverberation arc $>90^\circ$

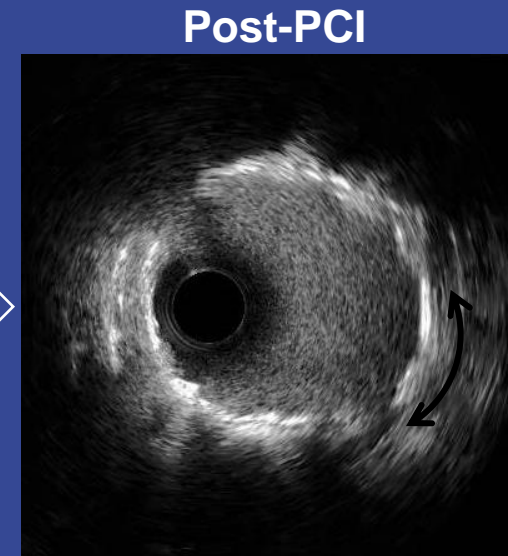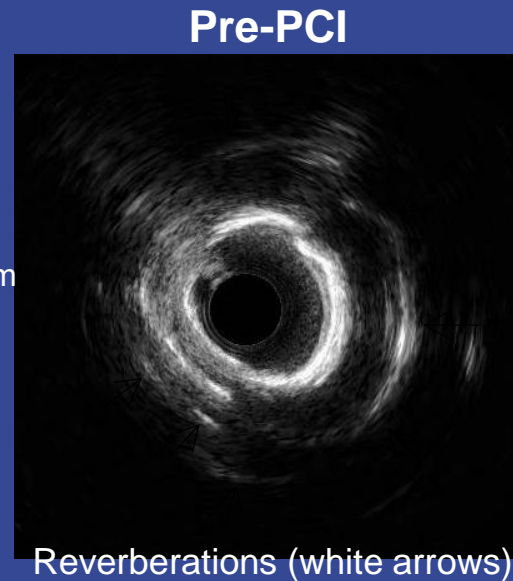


Excellent expansion despite severe Ca
Stent area= 9.7mm²

Note Ca fracture (newly visible perivascular tissue, double-headed white arrow)

	Cut-off value	AUC	Score
Length of Calcium $> 270^\circ$ (per 5mm)	5.4	0.73	$\leq 5\text{mm} \rightarrow 0$ point $> 5\text{mm} \rightarrow 1$ point
Vessel diameter (per 1mm)	3.4	0.74	$> 3.5\text{mm} \rightarrow 0$ point $\leq 3.5\text{mm} \rightarrow 1$ point
Calcified nodule	NA	NA	Absent $\rightarrow 0$ point Present $\rightarrow 1$ point
Reverberation arc (per 90°)	97°	0.81	$> 90^\circ \rightarrow 0$ point $\leq 90^\circ \rightarrow 1$ point

IVUS-Based Calcium Scoring System


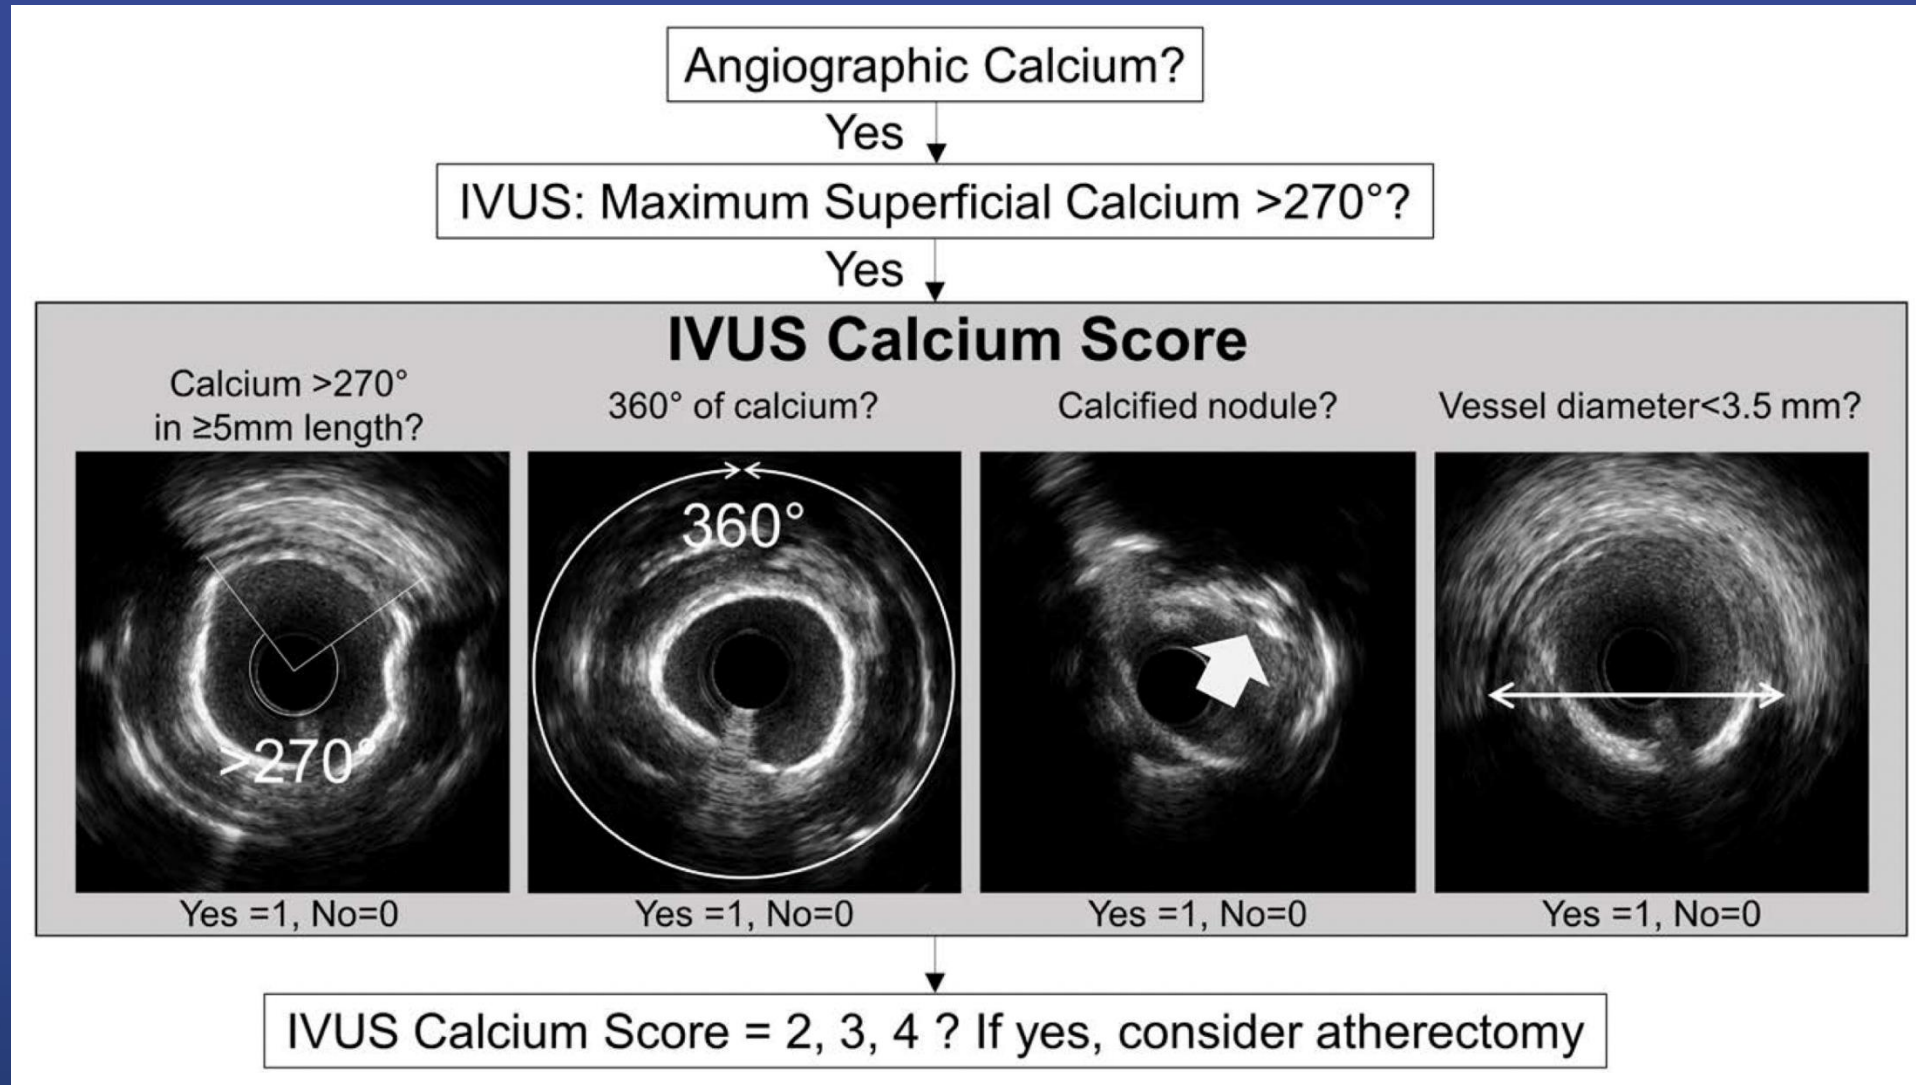


Calcium Scoring System (examples)

Case 1

- Length of Ca $>270^\circ$ = 4.1 mm = 0
- 360° of Calcium (+) = 1
- Calcified nodule (-) = 0
- Vessel diameter = 4.4 mm = 0



➔ **Calcium Score = 1**

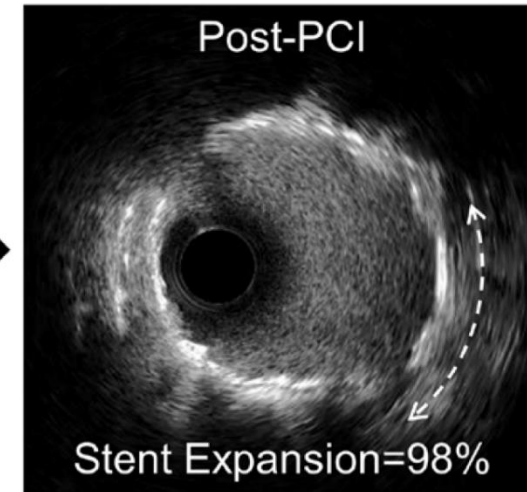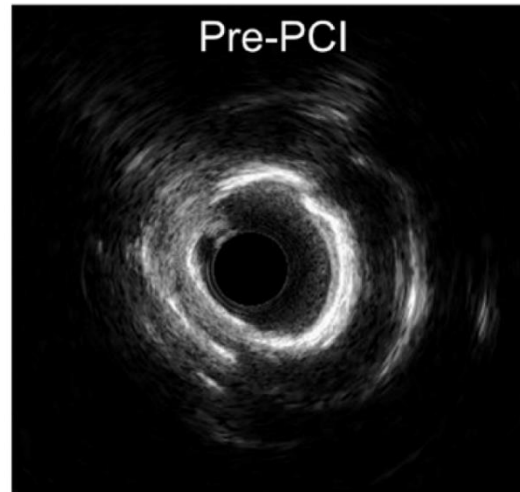

Case 2

- Length of Ca $>270^\circ$ = 8.9 mm = 1
- 360° of Calcium (-) = 0
- Calcified nodule (+) = 1
- Vessel diameter = 2.9 mm = 1

➔ **Calcium Score = 3**

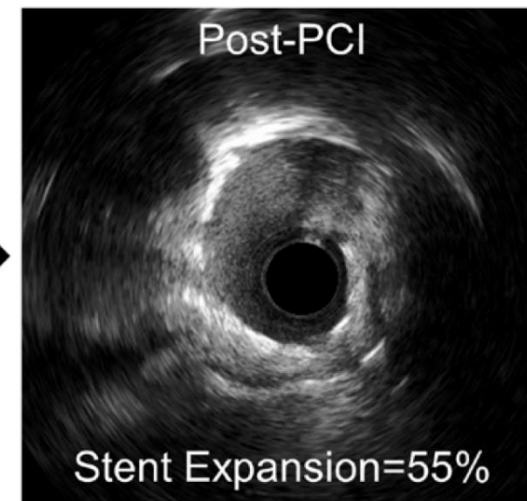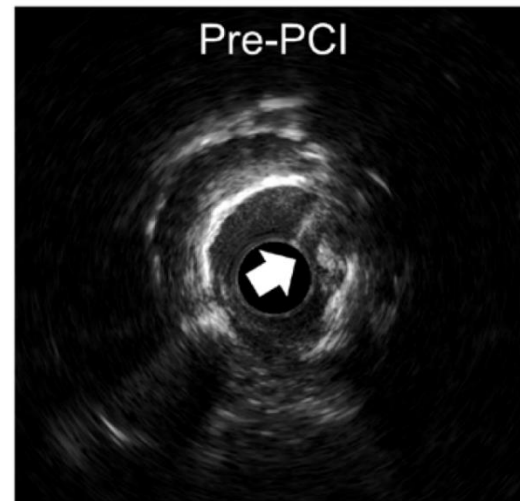

Angiosculpt Balloon


AngioSculpt is a scoring balloon catheter comprised of two main components:

1. Angioplasty balloon catheter

- semi-compliant nylon balloon
- coaxial, nylon shaft
- 2 marker bands

2. Scoring element

- laser-cut nitinol hypotube
- helical configuration

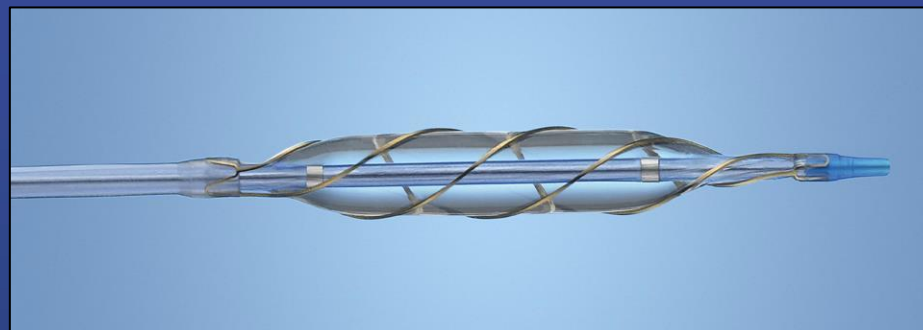


Scoring Mechanism of Action

AngioSculpt is the only device to offer 3 distinct benefits with one device:

- Precision
- Predictable Power
- Safety




Precision – Minimal Slippage

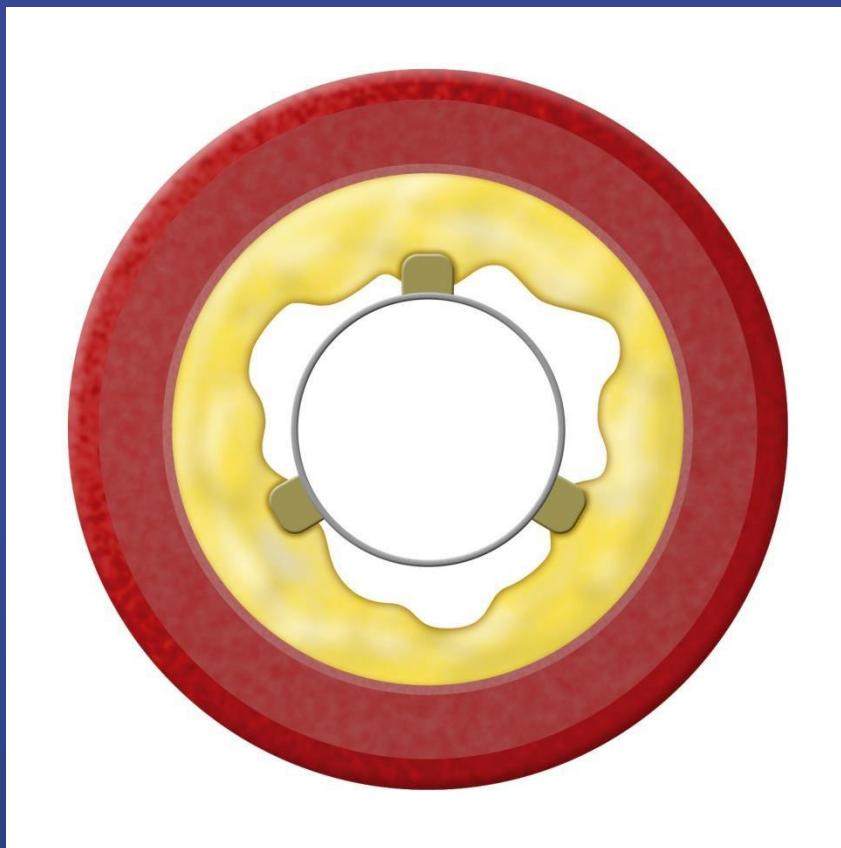

- Rectangular edges “lock” the device into lesion
- No significant device slippage = less damage to healthy tissue


Power – More Dilatation Force

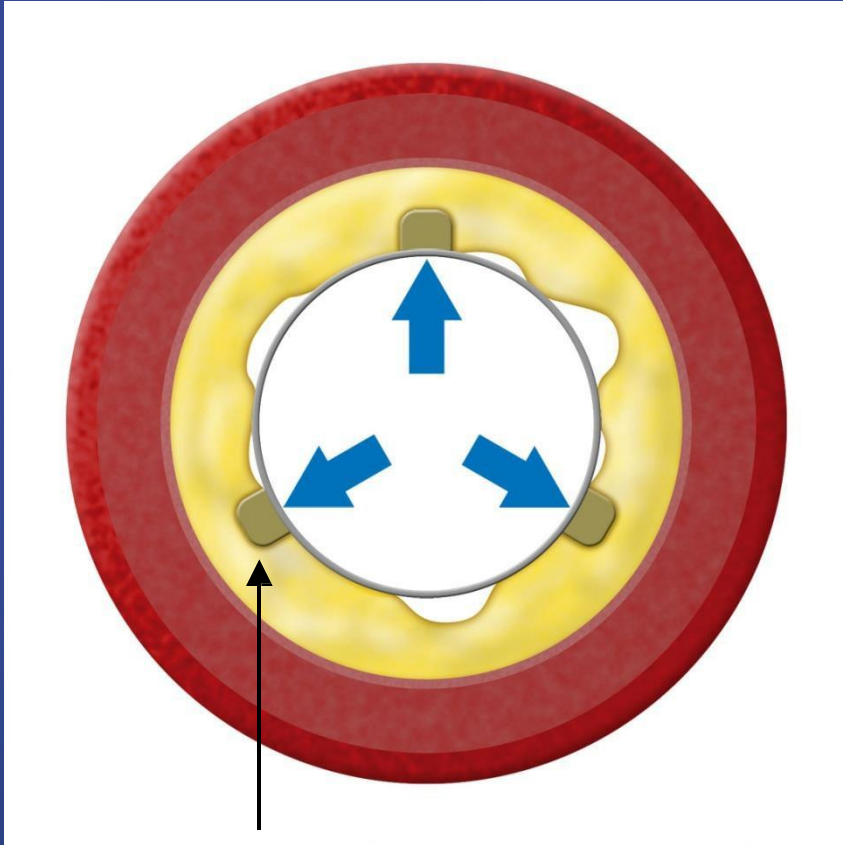

15-25X force of POBA*

- Leading edges drive outward force 15-25 times that of POBA
- Helical arrangement of scoring element creates uniform luminal enlargement

Safety – Low Dissection Rate

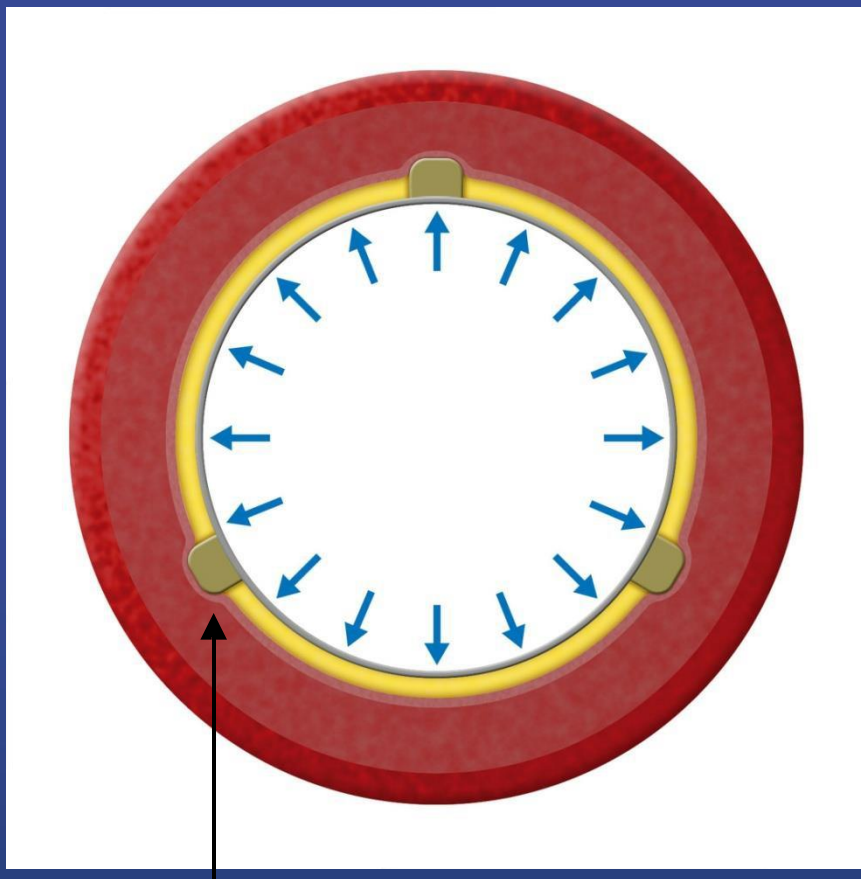

1X force post scoring*

- Post-scoring, outward forces are designed to be equivalent to POBA
- Low dissection rate
- Low rate of adjunctive stenting

Features & Benefits - Scoring Element


Feature	Benefit
<ul style="list-style-type: none">• Nitinol material	<ul style="list-style-type: none">• Facilitates balloon deflation
<ul style="list-style-type: none">• Helical shape	<ul style="list-style-type: none">• Uniform, circumferential scoring• Reduces balloon slippage
<ul style="list-style-type: none">• Electropolished rectangular edges	<ul style="list-style-type: none">• Provides safe scoring – minimize dissections



Element strut height

.005" or .007"


Cutting Balloon

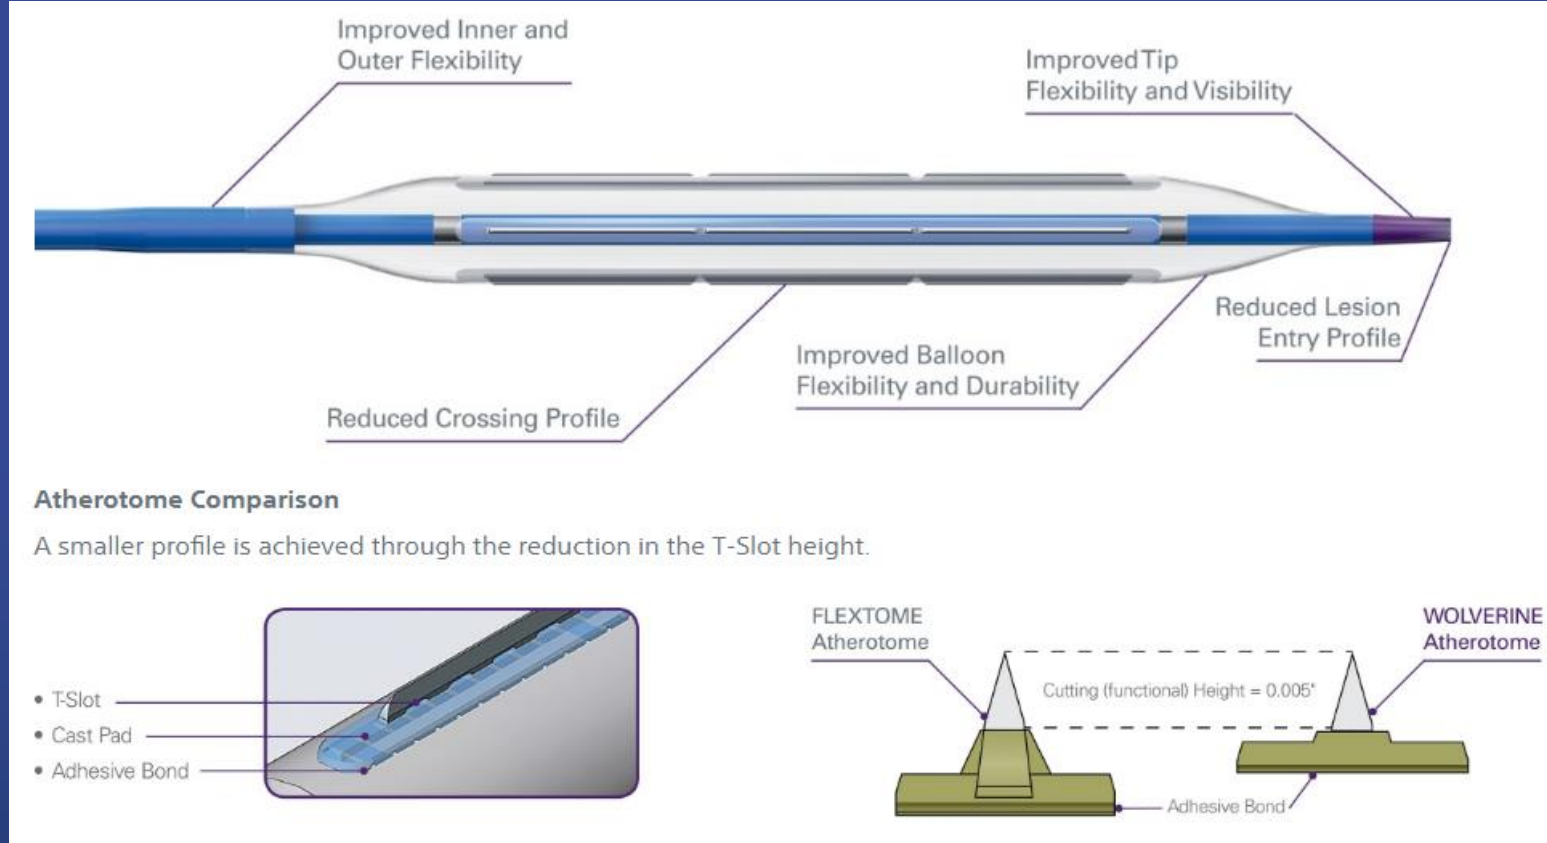

Cutting Balloon to Optimize Predilation for Stent Implantation: The COPS Randomized Trial

- 100 consecutive patients with calcified lesions
- Randomized to cutting balloon vs. non-compliant balloon
- Lesions excluded
 - In-stent restenosis
 - Graft restenosis
 - Thrombotic lesions
- Lesion characteristics
 - RVD 3.4 mm
 - Average calcium length: 12 mm
 - B2/C 71%

Cutting Balloon to Optimize Predilatation for Stent Implantation: The COPS Randomized Trial

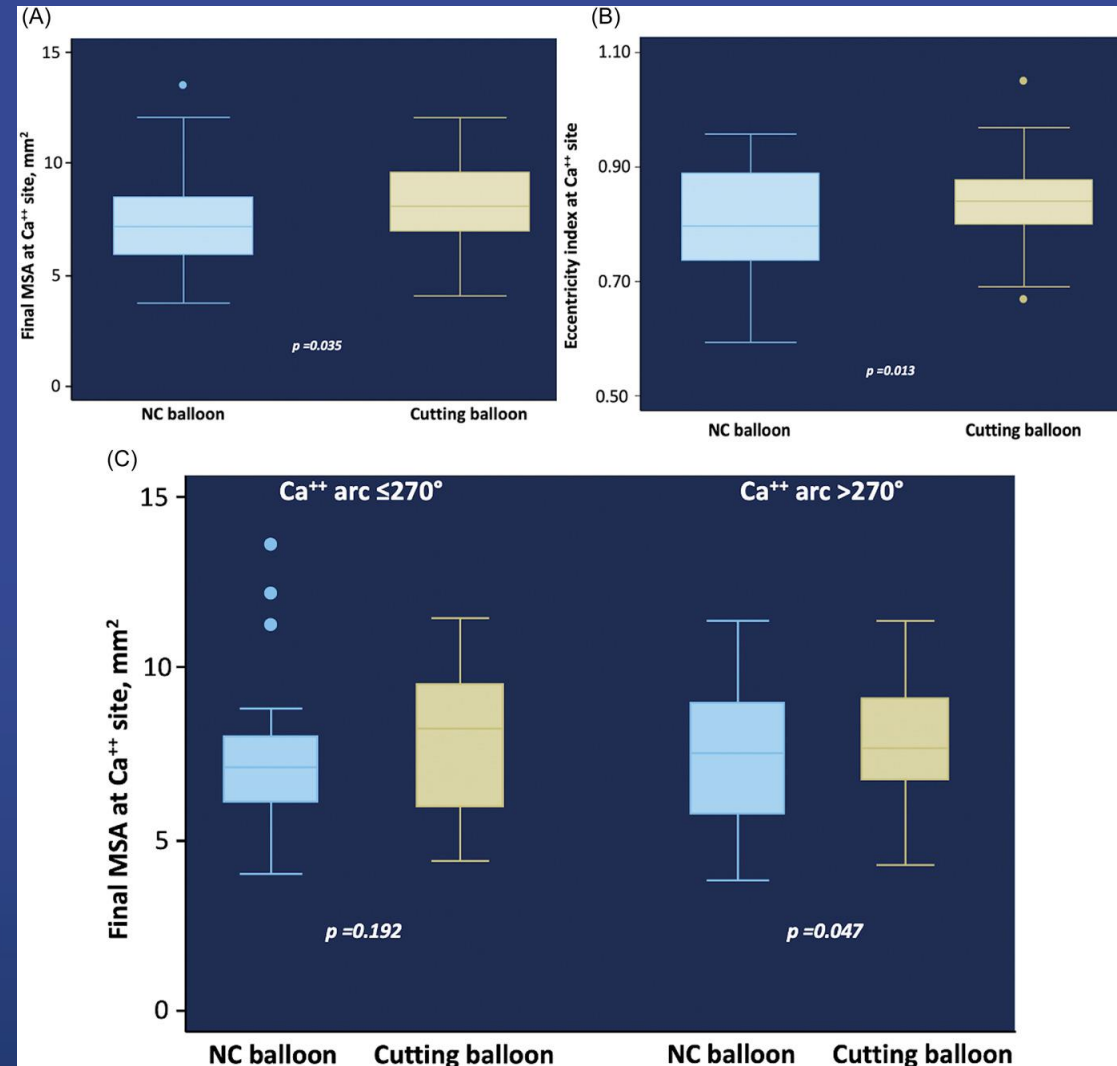

Israeli Registry -Baseline Characteristics

- 521 consecutive patients scheduled for PCI
- 521 patients and 745 lesions treated
- Lesions excluded
 - Without calcification
 - With untreated visible thrombus
- Lesion characteristics
 - RVD 2.48 mm
 - Average lesion length: 19.2 mm
 - Moderate/severe calcification: 75%
 - B2/C 53%
 - Bifurcations 18%
 - Angulated 43%

Israeli Registry – Results (Acute)

	Pre-ASC	Post-ASC	Post-Stent
MLD (QCA) mm	0.22 ± 0.17	2.04 ± 0.57	2.49 ± 0.69
DS%	84.8 ± 13.9	21.7 ± 12.7	5.7 ± 2.4
CSA (IVUS) mm ²	2.49 ± 0.39	3.72 ± 1.12*	5.30 ± 2.05*


*p<0.001

- Device slippage 1.2% lesions (9/745)
- Significant dissection (≥ type C) post ASC 1.5%
- No device-related perforations


Rotational Atherectomy or Balloon-Based Techniques to Prepare Severely Calcified Coronary Lesions

Patients With Severely Calcified Coronary Artery Lesions Amenable to Drug-Eluting Stent Implantation and Enrolled in the Randomized PREPARE-CALC and ISAR-CALC Trials (N = 274)


Patients with available OCT imaging after stenting included in the pooled analysis (n = 200)



Rotational atherectomy, n = 63



Modified balloon, n = 103




Super high-pressure balloon, n = 34

Main outcomes				Main findings
Stent expansion, %	73.2 ± 11.6	70.8 ± 13.6	71.8 ± 12.2	No significant difference
Maximal stent eccentricity	0.70 ± 0.06	0.70 ± 0.08	0.74 ± 0.09	Super high-pressure balloon better
Strategy success, %	100	86.4	91.2	Rotational atherectomy better

Rotational Atherectomy or Balloon-Based Techniques to Prepare Severely Calcified Coronary Lesions

FIGURE 3 Stent Eccentricity, Acute Lumen Gain, and Strategy Success According to Lesion Preparation Strategies

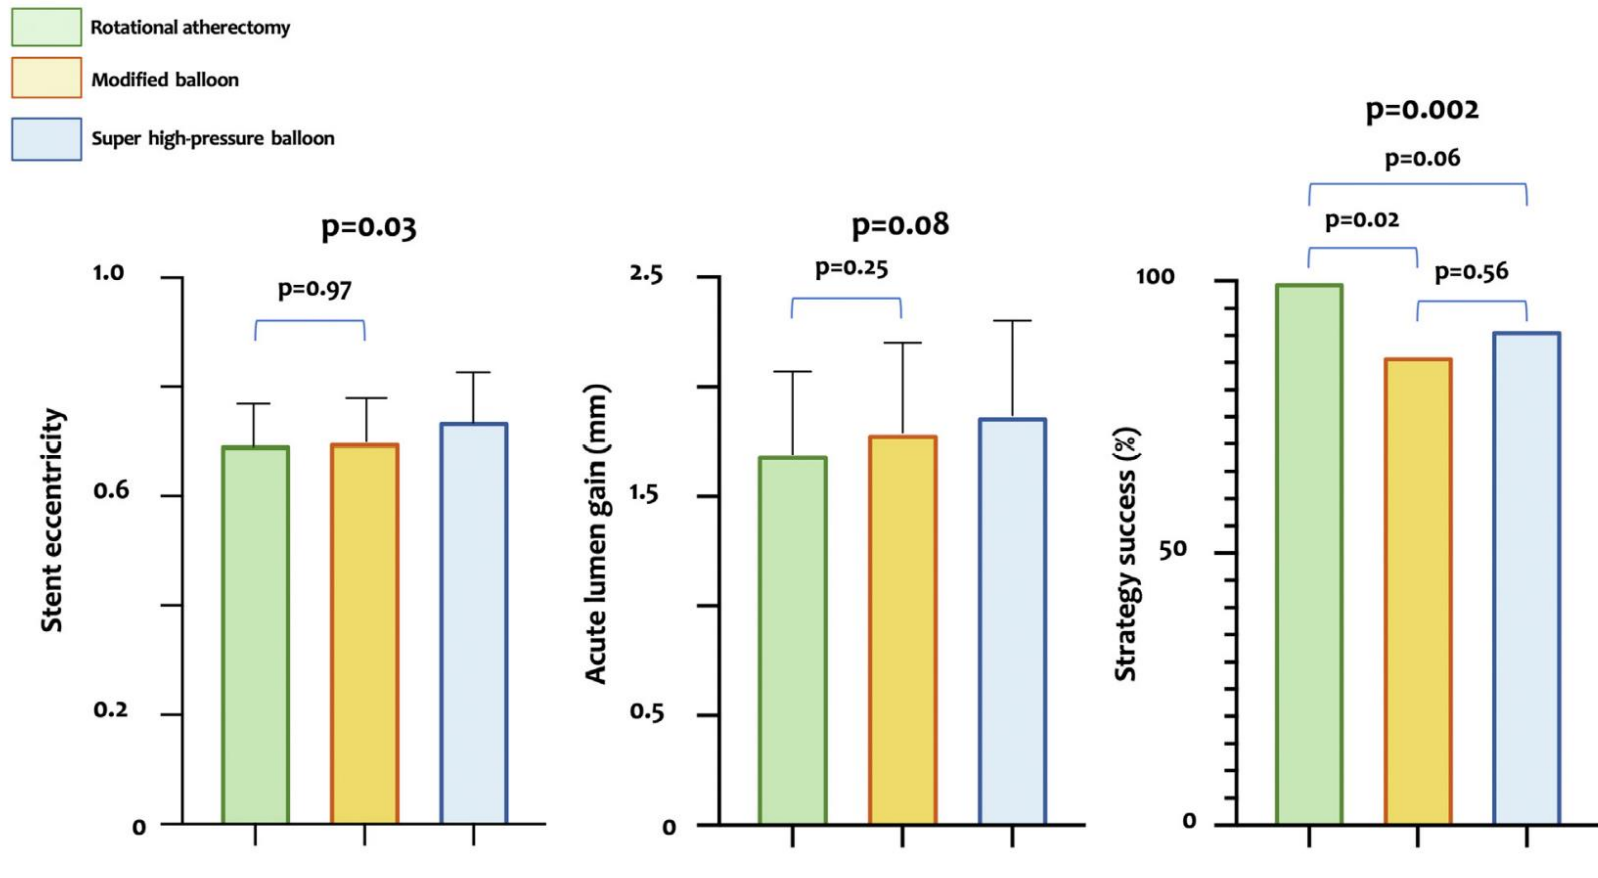


The height of the bars and the error bars display means and SDs, respectively.

Rotational Atherectomy (Rotablator)



- Burr : covered with 20-30 um diamond chips
- Guidewire : 0.009 inch with 0.014 inch tip

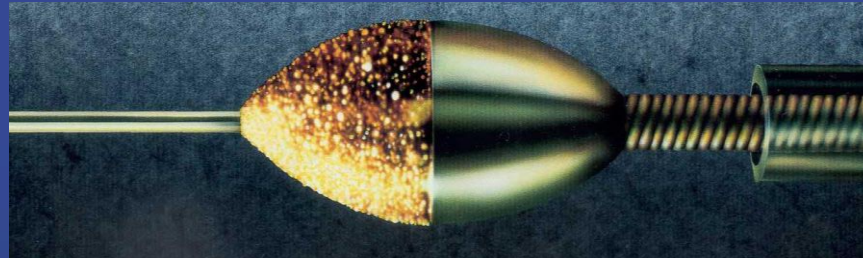


Rotablator Rotational Atherectomy System

FDA approved May 1993




Rotalink and Burr

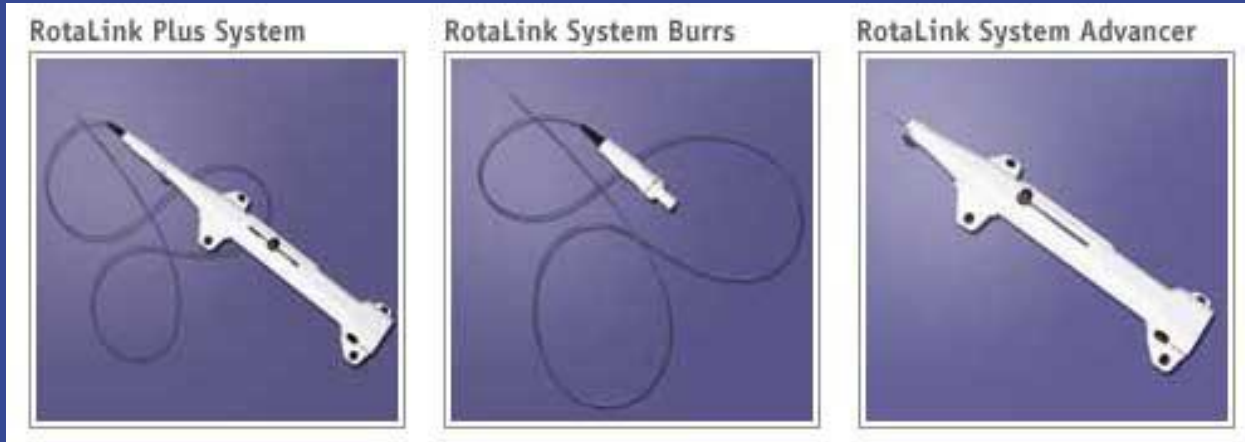


Pre-assembled

Separated

Diamond coated burr: 1.25 mm - 2.5 mm (0.25 mm increments)

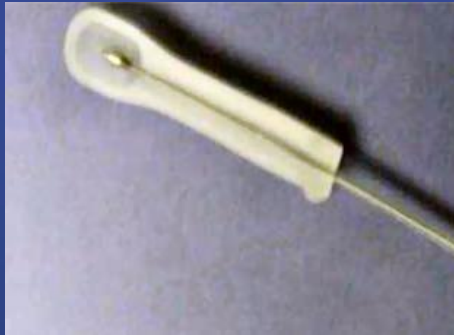

To avoid damage to the burr, **remove distal gripper** after connection to Advancer



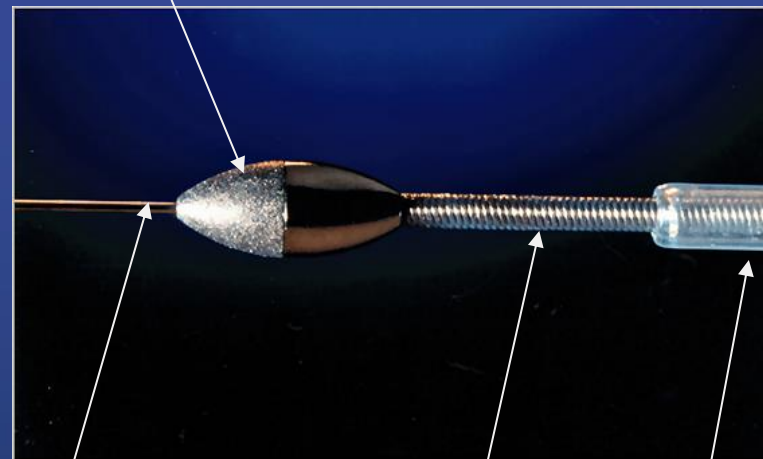


Rota-wire

Drive shaft

Sheath: 4.3 F O.D.

Console, Foot pedal, Gas, and Fluid

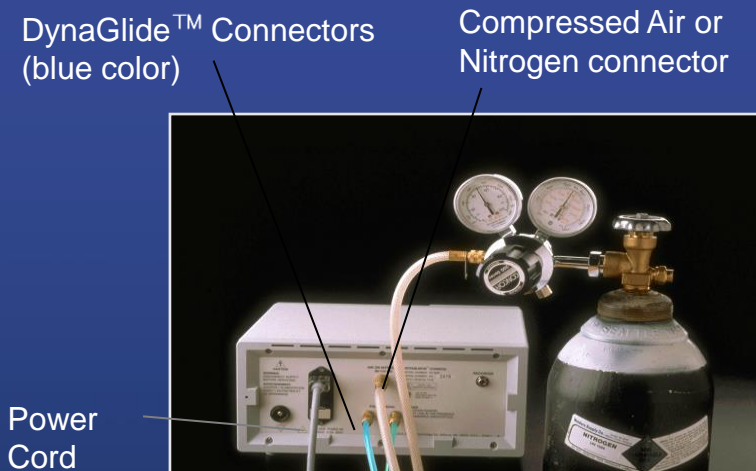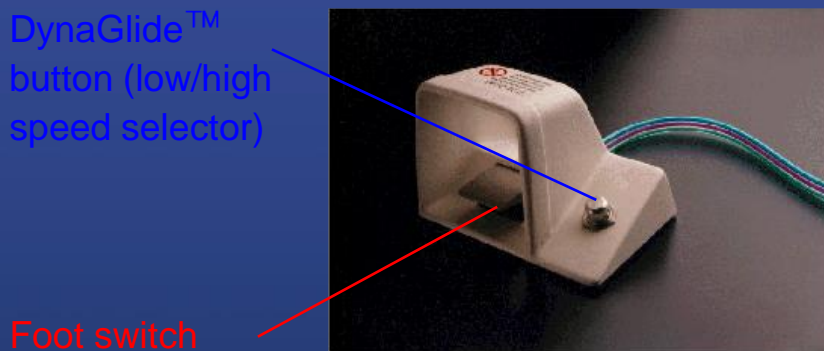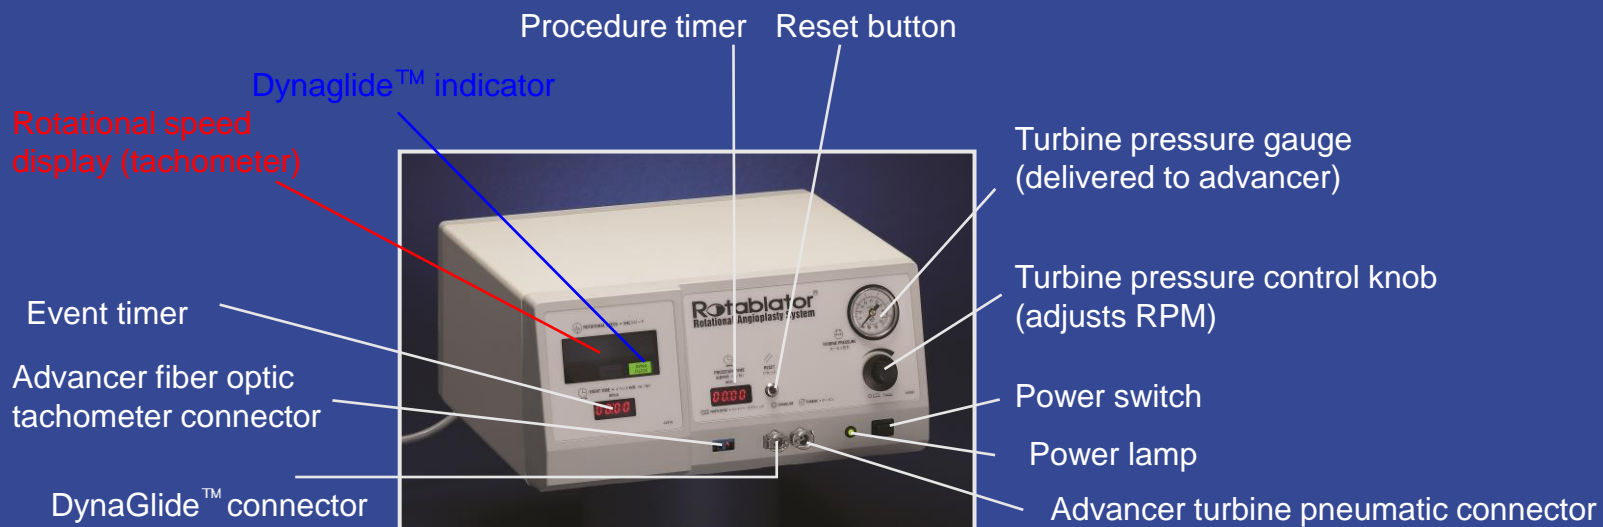


Rotawire

RotaWire floppy guidewire



- Tip diameter= 0.014 inch, body diameter= 0.009 inch
- Spring tip length = 22 mm
- 'Long neck' segment: 130 mm, 0.005 – 0.0077 inch
- Total length 3300 mm

RotaWire extra support guidewire

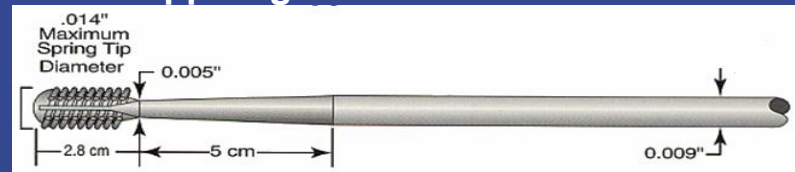

- Tip diameter= 0.014 inch, body diameter= 0.009 inch
- Spring tip length = 28 mm
- 'Short neck' segment: 50 mm, 0.005 – 0.0077 inch
- Total length 3330 mm


Cf) Rotalink length = 1350 mm

ROTAPRO™ Rotational Atherectomy System

ROTAPRO™ Console



ROTAPRO™ Advancer

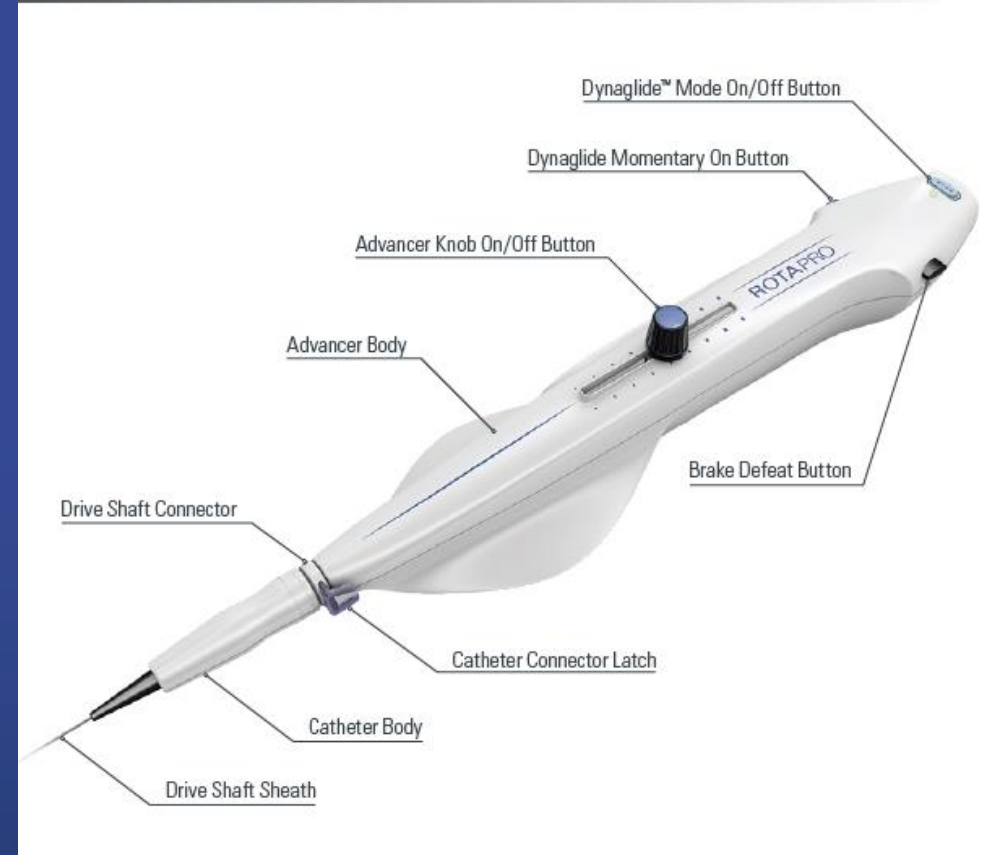


Current Indications of Rotablator

- **Indication: lesion modification**
 - Undilatable lesion or severely calcified lesion
 - Difficult to cross balloon or stent
 - Stent ablation

- **Relative contraindication**
 - Severe angulation
 - Extremely eccentric lesion
 - Vessel size is too small
 - Pre-existing severe dissection or vasospasm
 - High risk of no-reflow: thrombotic lesion, SVG

Principles of Rotational Atherectomy

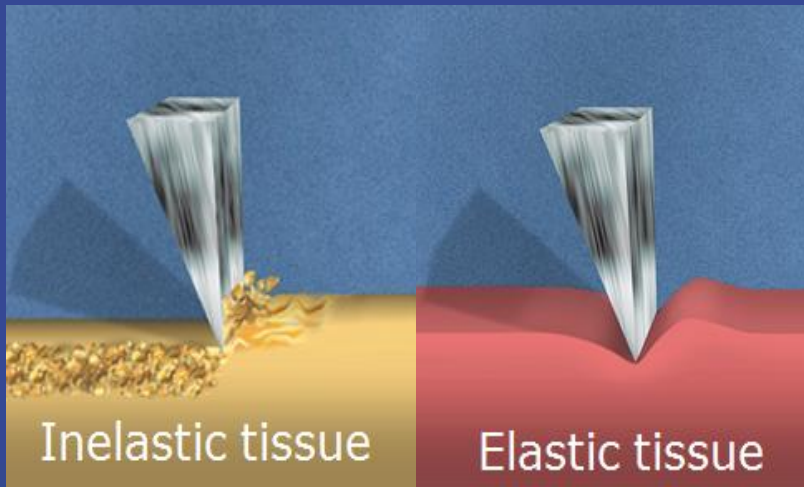


Differential Cutting



Orthogonal displacement
of friction


Microparticulate Debris

- Size: < 12 micron in 88%
- Increased size of debris when
 - Slow burr speed < 75,000 rpm
 - Deceleration by pushing hard > 5000 rpm

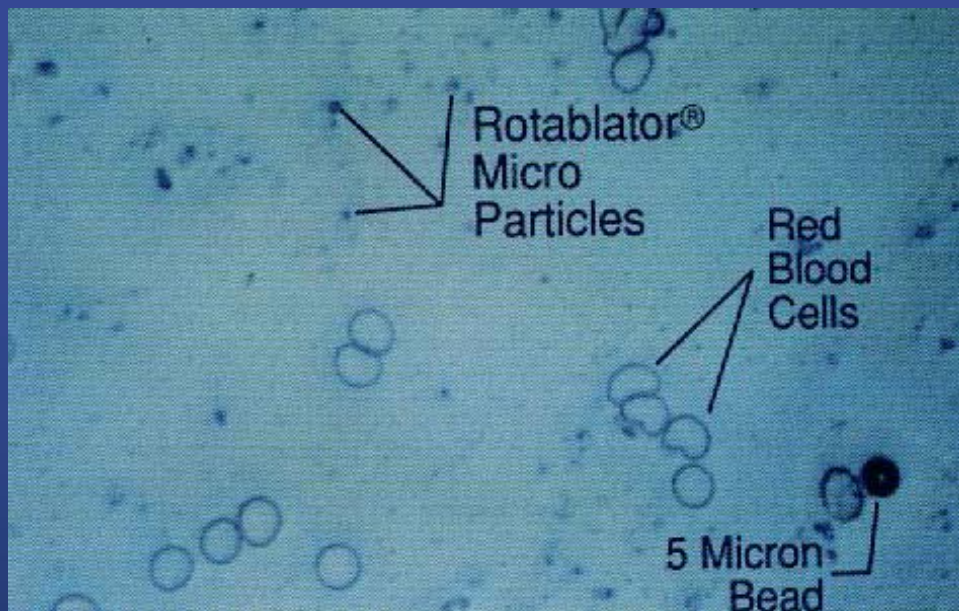

Burr Selection

- Burr-to-artery ratio: upto 0.5
- One-burr vs. two-burr approach
- Burr speed
 - Large burr (≥ 2.0 mm) : 150,000 rpm
 - Small burr (≤ 1.75 mm) : 180,000 rpm

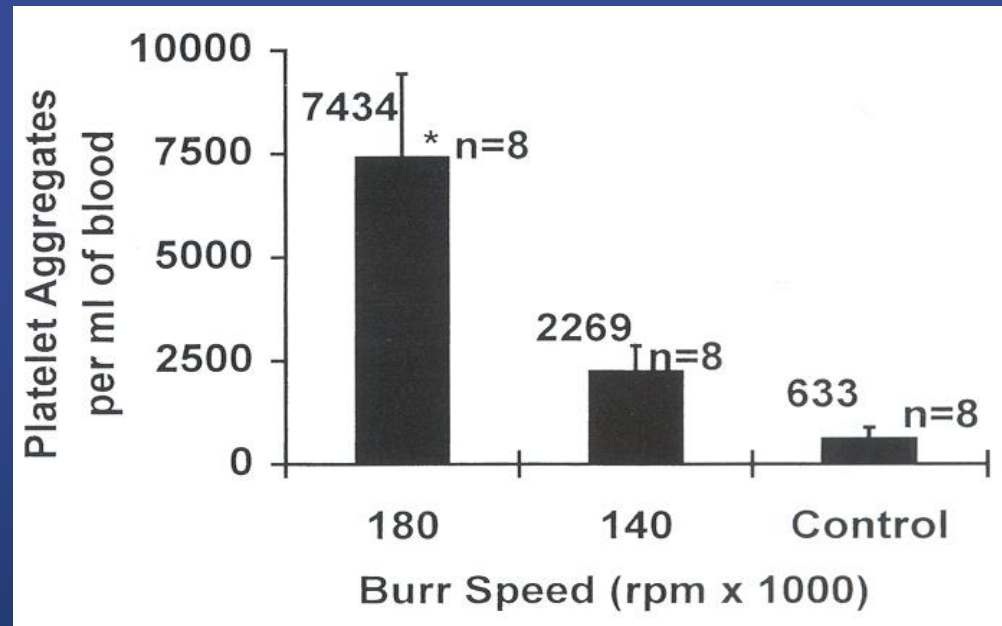

Reisman, Cath Cardiovasc Diag 1998

Burr Size and Guiding Catheter

Rotablator Burr Size (mm)	Burr Diameter Inches/mm	Recommended Guide Catheter (Fr)	Minimum ID (Inches/mm)
1.25	0.049/1.245	5-6	0.053/1.346
1.50	0.059/1.499	6	0.063/1.600
1.75	0.069/1.753	7	0.073/1.854
2.00	0.079/2.007	8	0.083/2.108
2.15	0.085/2.159	8	0.089/2.261
2.25	0.089/2.261	9	0.093/2.362
2.38	0.094/2.388	9	0.098/2.489
2.50	0.098/2.489	10	0.102/2.591


* Guiding catheters without abrupt primary or secondary curves are recommended (FR4, CLS, XB etc)

Cocktail solution

- Infused into Rotalink advancer by pressure-bag (50~100 mmHg above the blood pressure)
- Infusion speed 6-8 ml/30 sec
- Contents
 - Normal saline 500 ml
 - Nitroglycerin 2 mg
 - Heparin 2500 unit
 - Verapamil 5 mg
- Rotaflush study (Matsuo, AHJ 2007)
 - Nicorandil is better than verapamil in terms of ST resolution, and the risk of NQMI and QMI

Complications of Rotablation

- Slow or no-reflow
- Dissection
- Perforation
- Wire bias problems
- Lodged burr
- Spasm
- AV block

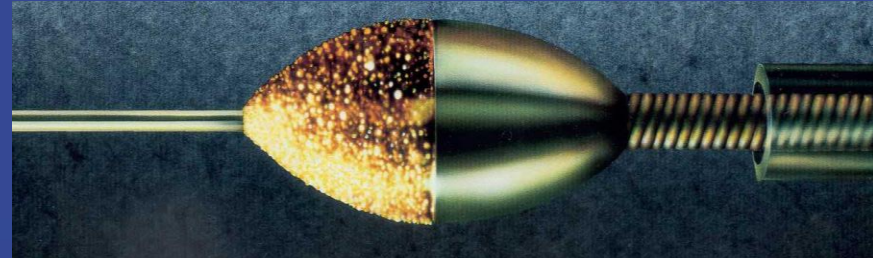

Slow Flow / No Flow

- Overview

- Slow flow and no flow are observed in 5% of patients undergoing PTCRA
- Slow flow is a diminution of flow by 1-2 TIMI grades from the baseline antegrade flow
- No reflow is a cessation of flow into the distal coronary bed

- Potential Course of Action

- Early recognition of flow disturbance is key
- Time
- IC Nitroprusside, verapamil or adenosine: careful of hypotension and bradycardia
- IABP if needed
- Intermittent injections of contrast media during ablation run for flow interrogation
- Appropriate burr run time for lesion and vessel complexity

Lodged Burr

- Causes

- Oversized burr in diffuse calcium and too much pressure can jam
- Small burr in eccentric lesion and too much pressure can cause watermelon seeding thru lesion and with no diamonds on proximal side of burr, no way to get back

- Potential Course of Action

- Do not attempt to start the burr spinning once it is stuck. Take an angiogram to determine burr position
- Nitro, cough and time
- DynaGlide™: Burp foot pedal while gently pulling catheter shaft. Brief spurt of energy and gentle pull back simultaneously
- Buddy wire with 1.5 mm ballooning if possible
- Pull the burr very hard, as the last resort!
- Surgery if required

AV Block

- Causes
 - No flow or slow flow for AV nodal branch
 - RCA > LCX > LAD
- Course of action
 - Cough CPR
 - Atropine
 - Temporary pacemaker


Incidence and Determinants of Complications in Rotational Atherectomy (J-PCI Registry)

In hospital death, cardiac tamponade, emergent surgery

	OR	95% CI	P Value
Age (1-y increase)	1.03	1.02–1.05	<0.001
Impaired kidney function	1.59	1.15–2.19	0.004
History of previous myocardial infarction	1.69	1.21–2.35	0.002
Emergent PCI	4.02	1.66–8.27	<0.001
Triple-vessel disease (vs single-vessel disease)	2.17	1.43–3.28	<0.001
Left main disease (vs single-vessel disease)	2.54	1.51–4.17	<0.001
High-volume institution (vs low-volume institution)	0.56	0.36–0.89	0.011





Kenichi, et al., *Circulation Intv.* 2016; 9: 11.

Intravascular coronary lithotripsy

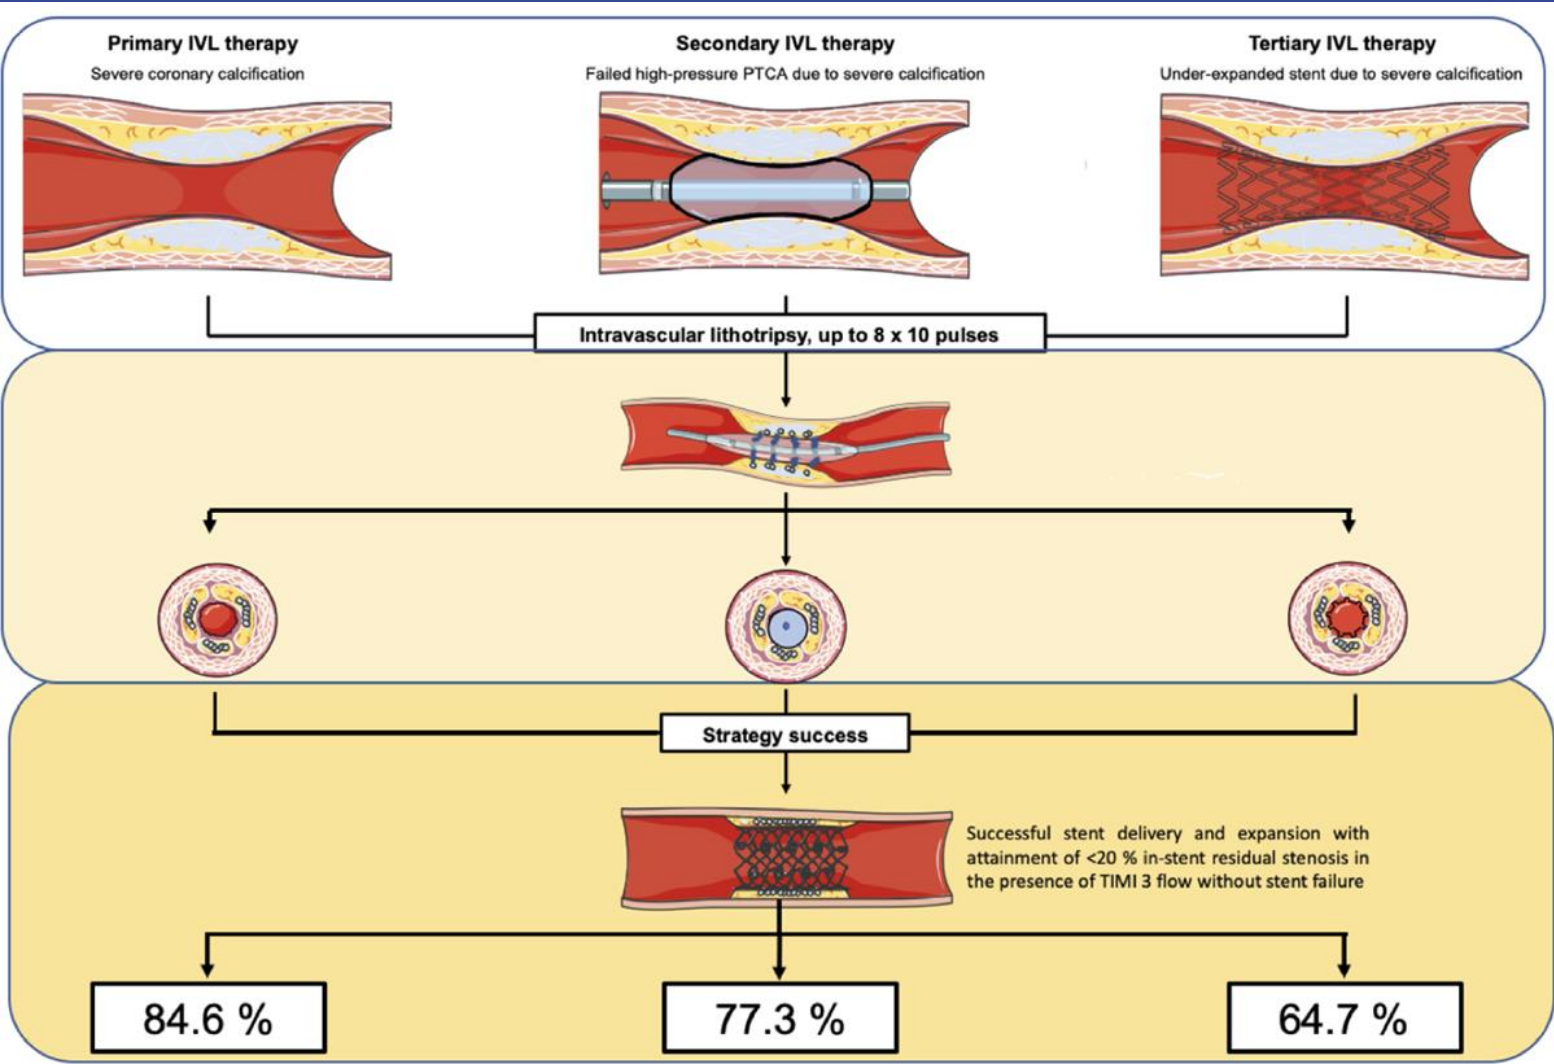

Intravascular coronary lithotripsy



Beneficial impact of IVL on calcium modification and stent expansion with low ID-TLR and stent thrombosis rates

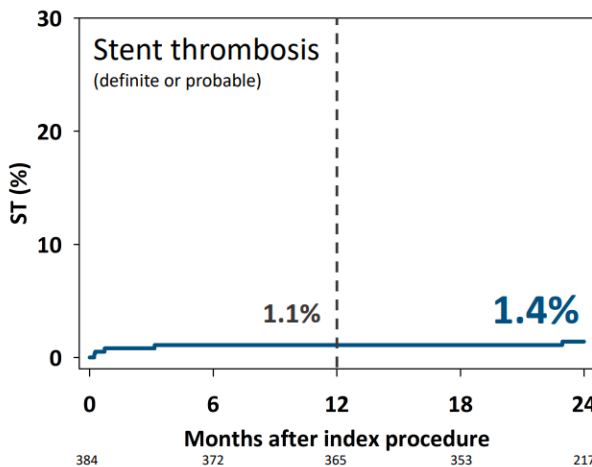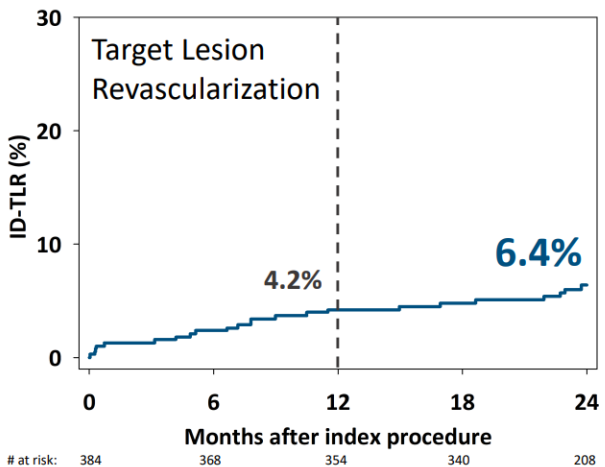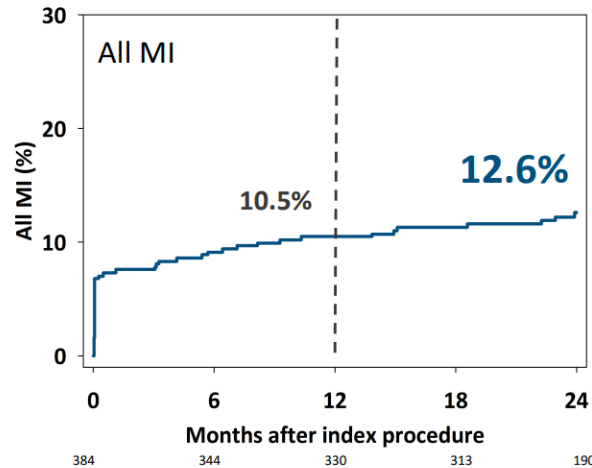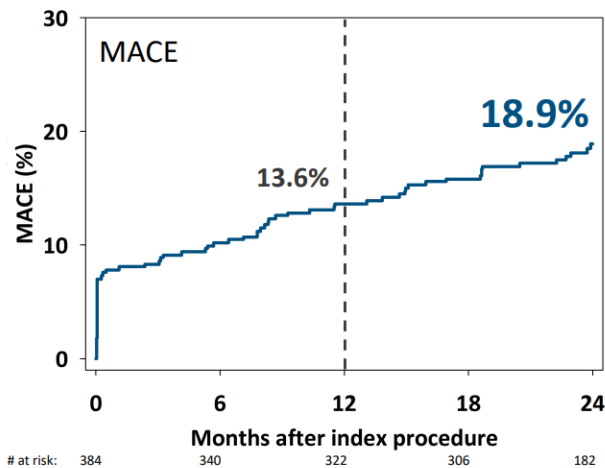

Beneficial impact of IVL on calcium modification and stent expansion with **low ID-TLR and stent thrombosis** rates - Final 2-year result from the Disrupt CAD III study

Intravascular coronary lithotripsy


CENTRAL ILLUSTRATION: Luminal Area Gain Following IVL Treatment and Stent Deployment

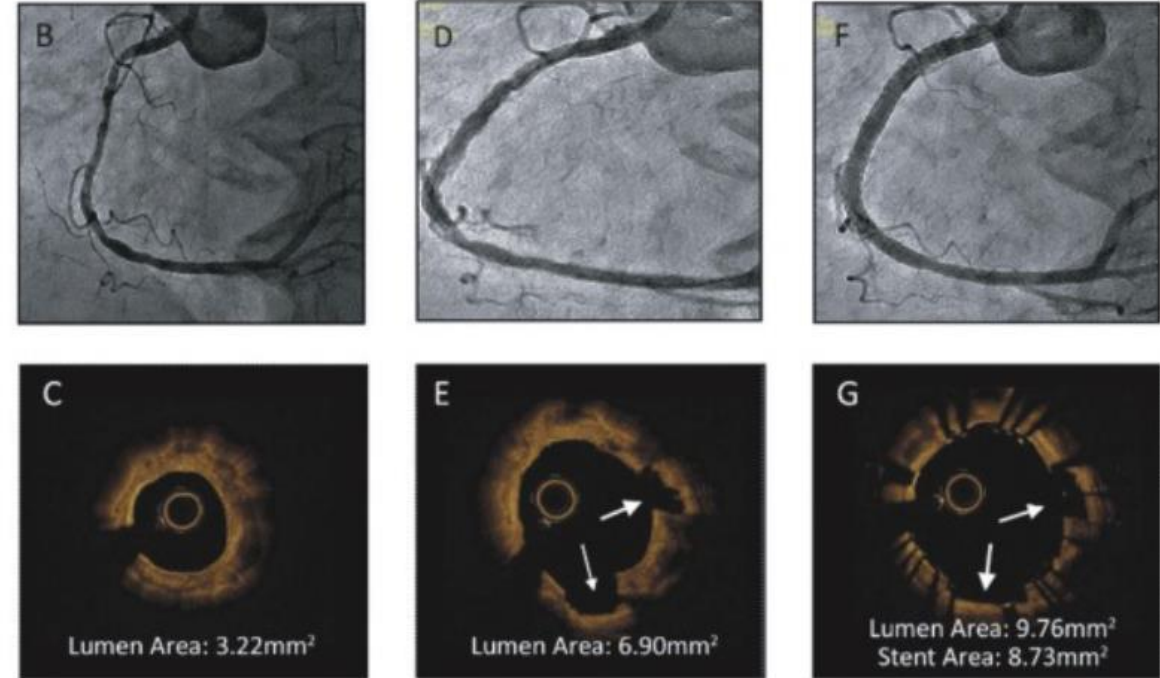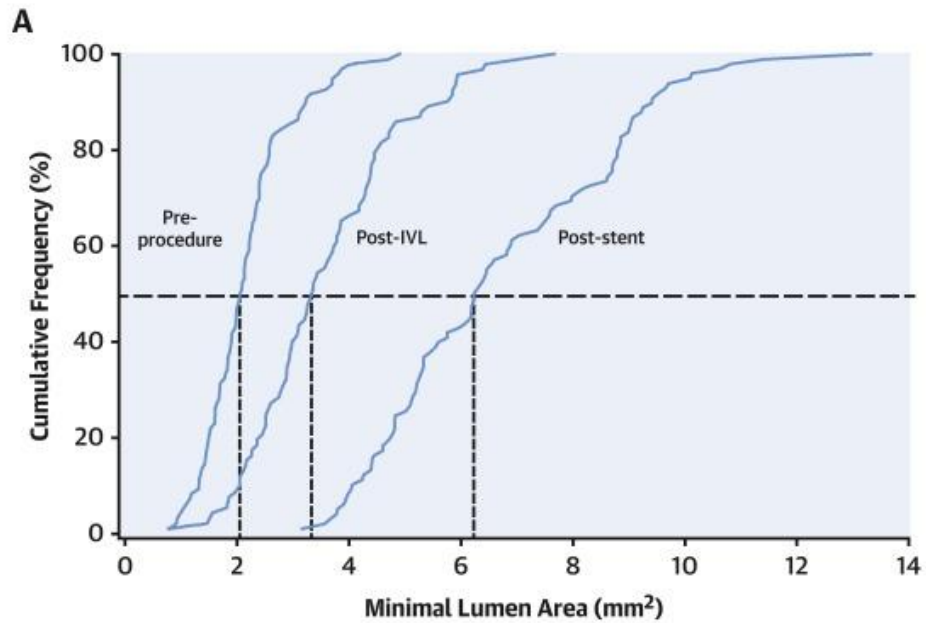

Coronary IVL safely and effectively facilitated stent implantation in severely calcified lesions

Technical Issues

Rotalink advancer

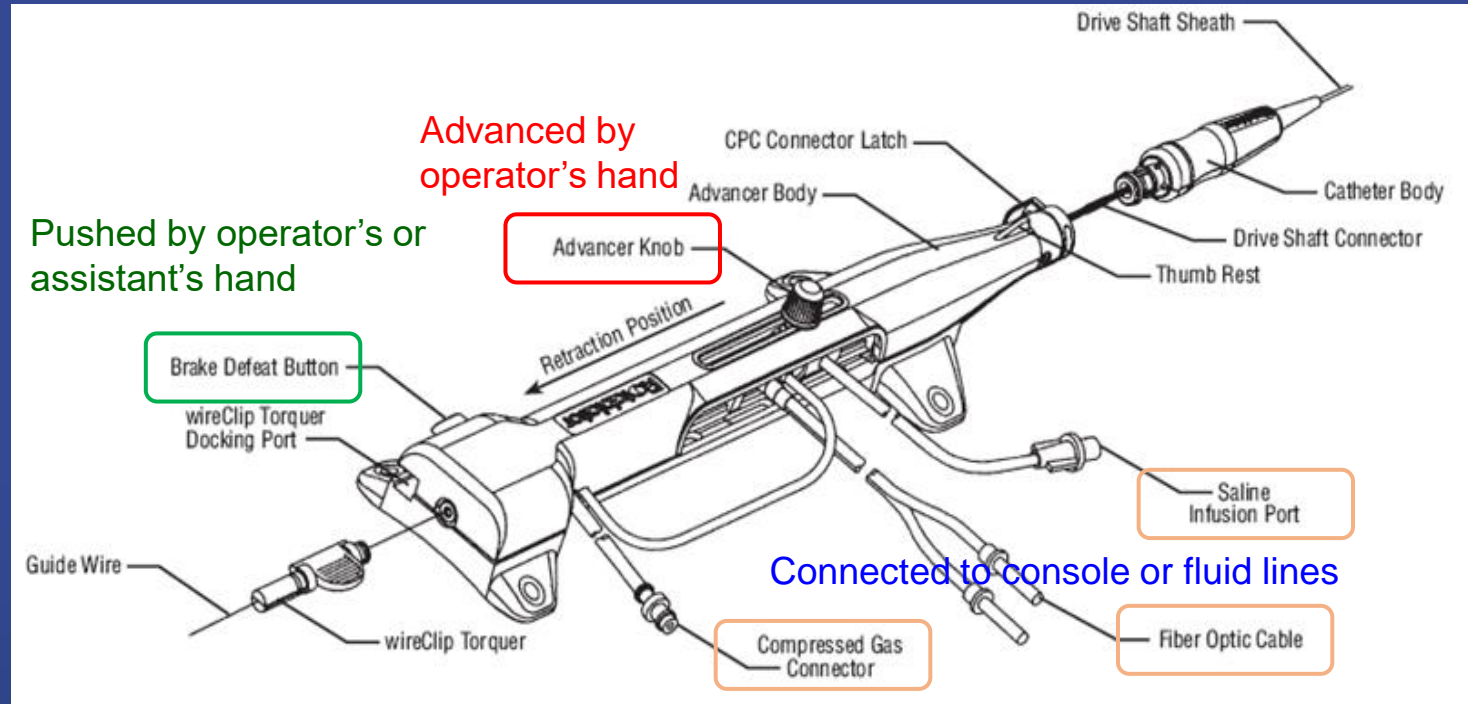


Basic procedural steps (1)

1. Place the rota-wire beyond lesion
 - Rota-wire is very delicate. No severe bends
 - Rota-wire has poor torque conduction. Use microcatheter or over-the-wire balloon to exchange with conventional guidewire.
2. Select burr size: Burr-to-artery ration $< 0.5 - 0.7$

3. Backload and advance assembled burr + advancer unit over rota-wire. Place wire clip at the end of rota-wire.




4. Lock advancer knob 2 to 3cm forward before advancing burr into guiding catheter. Turn on the flush solution and do brief RPM check while holding the Y-connector firmly.
 - It removes tension/inertia on the burr (sudden burr advancement or jump)
 - *(Cover the burr with wet gauze to prevent damage)*



Basic procedural steps (2)

5. Press Dynaglide button to activate Dynaglide mode (60,000 – 80,000 rpm).



6. Advance the burr to the 'landing zone' (non-stenotic site proximal to the lesion) in the proximal coronary artery

- Avoid tightening of Y-connector. The hemostasis valve should be closed just tight enough to prevent blood loss, but still allow the RotaLink Sheath to slide through the valve.

7. Remove residual tension/inertia of burr at landing zone

- Move advancer knob back and forth to remove tension between drive shaft and Teflon sleeve
- Release Y-connector and move burr back and forth to remove tension between guidewire and rota burr
- Brief Dynaglide run under fluoroscopic guidance. If there is residual tension/inertia, sudden burr advancement or jump occurs.

Basic procedural steps (3)

8. Basics of rotablation

1. Burr motion: To-and-fro pecking motion > slow advancement
2. Burr run time: the shorter is the better, 15–20 sec
3. Burr speed: the higher is the better, > 180,000 rpm*
4. Advance burr no more than 3 cm back and forth. Moving forward only when there is light resistance.
5. Avoid running the burr in static position. Always keep the burr advancing or retracting while it is rotating.
6. Avoid significant drop in rpm (> 5000 RPM for > 5 sec)
7. Aggressively keep blood pressure and heart rate.
8. Do final 'polish run' (no rpm drop, no resistance) after completion of rotablation.
9. Long lesions were divided into segments and each segment was separately ablated.

Basic procedural steps (4)



9. Get feedback of rotablation

- Tactile: advancer knob resistance or driveshaft vibration
 - excessive load on burr
 - too rapid advancement
 - a kink in the drive shaft coil
 - too large burr
- Visual: smooth advancement under fluoroscopy
- **Auditory**: Pitch changes relative to resistance encountered by the burr

Basic procedural steps (5)

10. Tips for successful rotablation

1. Never adjust RPMs during ablation.
2. Do not over-tighten Y-adapter.
3. Avoid dottering.
4. Avoid burring in the guide catheter (except Dynaglide mode).
5. Gently advance or retract the burr while it is at high speed rotary motion.
6. **Never stop burr in lesion or distal to lesion.** Burr should be located at the proximal 'landing zone' or within guiding catheter when not running.
7. Do not allow the burr to remain in any location while rotating at high speeds. **Always keep the burr advancing or retracting while it is rotating.**
8. Never advance rotating burr to point of contact with the guidewire spring tip. The guidewire can be destructed easily.

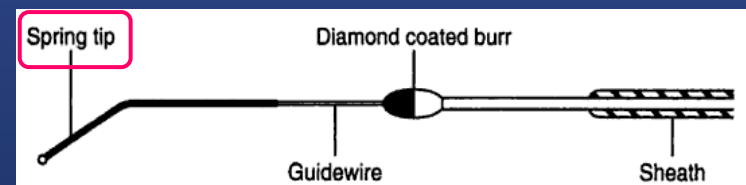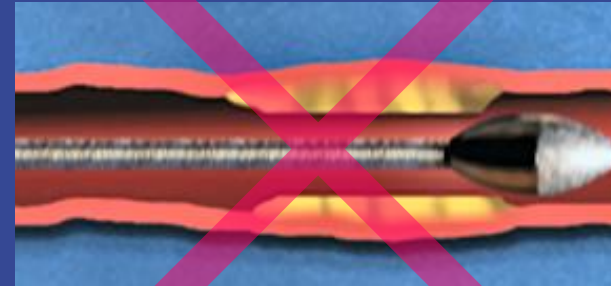

Procedure

1. Place the rota-wire beyond lesion
Easy to bend, poor torque control
Use microcatheter or OTW balloon for wire exchange
2. Select burr size: Burr-to-artery ration ≈ 0.5
3. Backload and RPM check
150K RPM for 1.75 or larger burr, 180K for smaller burr
4. Advance the burr upto landing zone (with or without dynaglide)
5. Tension release and dye injection
6. Start ablation
 - 1) Burr motion: To-and-fro pecking motion for 15~20 sec
 - 2) Never stop burr in lesion or distal to lesion
 - 3) Get feedback: visual, auditory for drop in rpm > 5000 RPM for > 5 sec
 - 4) Intermittent dye injection for slow flow
 - 5) Polish run after cross
7. Remove burr using dynaglide

DIAMONDBACK 360: Coronary Orbital Atherectomy System

Device Features

- Simple device setup
- Microsecond feedback to changes in loading
- 135cm usable length

On-handle speed control

- Low (80K) and High Speed (120K)

Power on/off switch

- 8 cm axial travel

Electric motor powered handle

Eccentric diamond coated crown

6Fr Guide Compatible

Saline Infusion Pump

- Mounts directly on to an IV pole
- Provides power
- Delivers fluid
- Includes saline sensor

ViperSlide® Lubricant

- ViperSlide reduces friction during operation
- 20ml ViperSlide per liter of saline

0.012" Viper Wire




Orbital atherectomy



A DEEPER LOOK

Differential Sanding⁴

The diamond-coated crown sands intimal calcium into particulate with an average size of approximately 2 μm – which is smaller than a capillary vessel.




Pulsatile Forces¹⁻⁴



The pulsatile impact of the crown may facilitate fracture of deep calcium.

Procedural Safety⁵

With the Diamondback 360[®] Coronary Orbital Atherectomy System, healthy tissue safely flexes away from the crown during operation, reducing impact to the medial layer. The orbital movement of the crown allows blood and saline to flow continuously during procedures, minimizing risk of thermal injury and slow flow/no reflow events.




Laser atherectomy

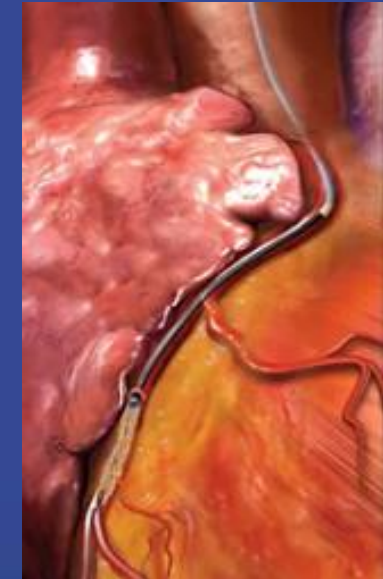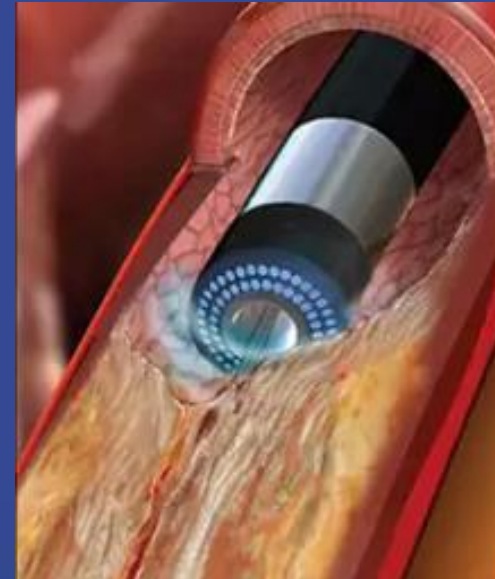

PHILIPS Coronary laser atherectomy catheter

Guidezilla II

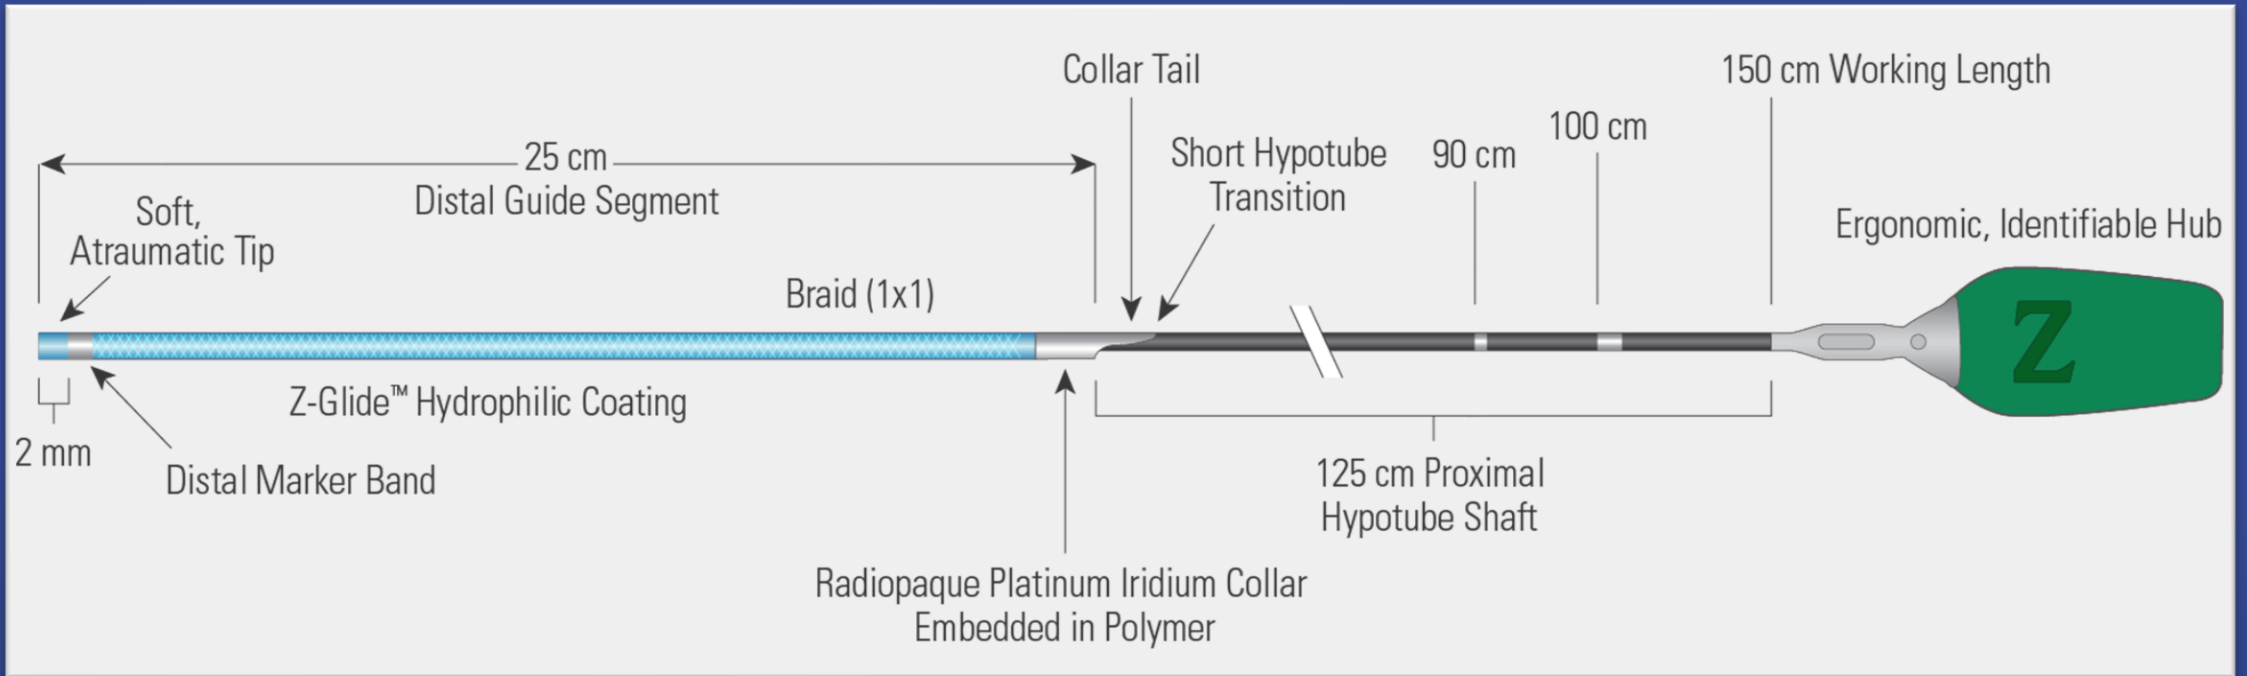

Guidezilla II

Powerful Reach. Predictable Performance.

Short Hypotube Transition
for reduced device
interaction

Radiopaque Helical Collar
Designed for improved
strength and visibility

Z-Glide™ Coating
For improved
deliverability

Green Ergonomic Hub
Unique and easily
identifiable




Expanded Size Matrix
6, 7 & 8F 25 cm;
6F 40cm
(Rapid Exchange
Length Noted)

Design Changes

(Guidezilla to GUIDEZILLA™ II)

Features	Guidezilla	GUIDEZILLA II	Design Goal
Sizes	6F	6F, 7F, 8F, and 6F Long	Expanded Size Matrix
Guide Segment	25 cm	25 cm on 6F,7F,8F (40 cm on 6F Long)	40cm 6F Long Designed for TRI
Working Length	145cm	150cm	Extra 5 cm Proximal Hypotube Shaft
Collar	Stainless Steel	Helical Platinum Iridium	Visibility, Strength, and Smooth Device Interaction
Coating	Bioslide™	Z-Glide™	Deliverability
Radiopaque	Distal Marker Proximal Marker	Distal Marker band Radiopaque Collar	True Device Positioning with Added Visibility
Hypotube Transition	19mm	6mm	Optimized to Reduce Device Interaction
Hub Design			

Guidezilla

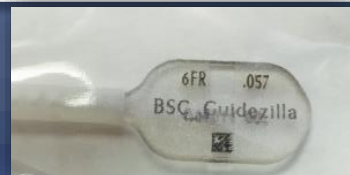

GUIDEZILLA II

GuideLiner

GuideLiner®

V3 Catheter


Beyond Tried. True.



Coaxial alignment and backup support




Deep-seating for distal device delivery

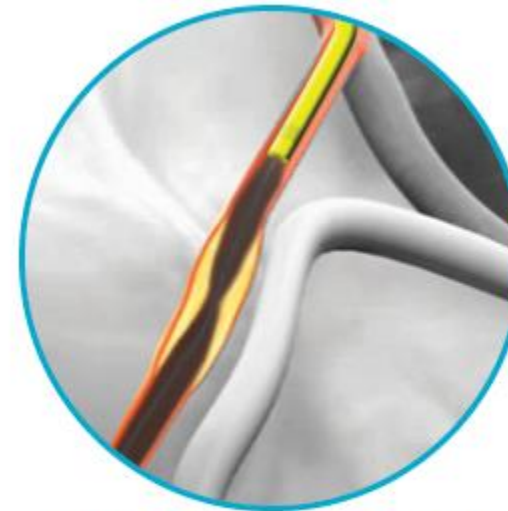

Selective delivery of contrast

Telescope

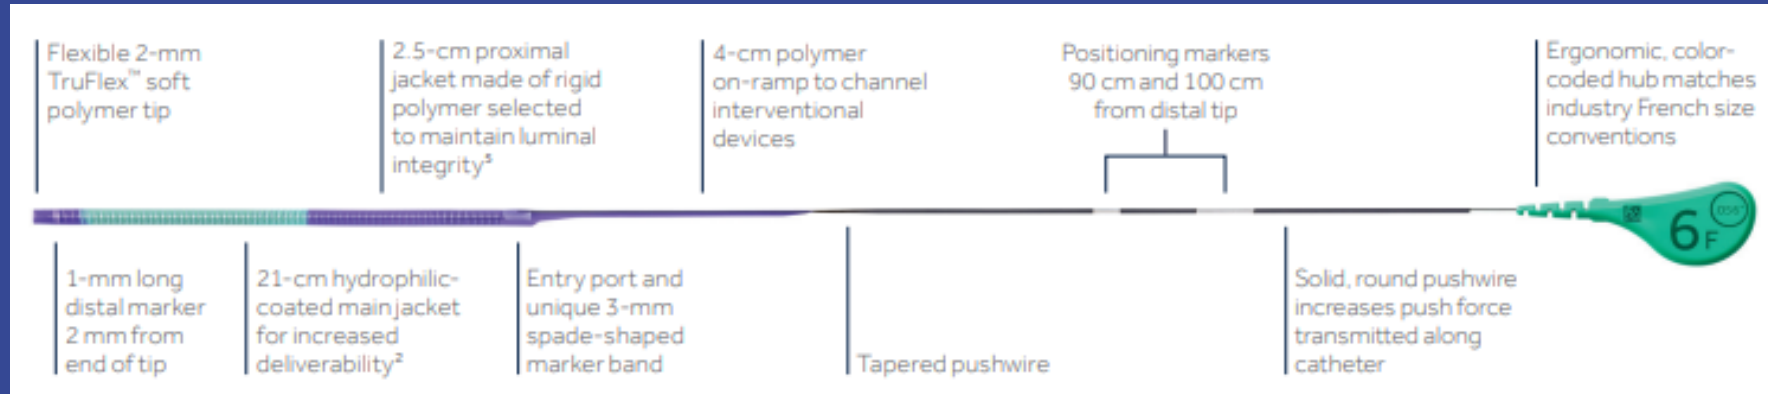

TECHNICAL FEATURES



Technical Features	Telescope™ GEC
Catheter length	150 cm
Distal extension length	25 cm
Marker band material	Platinum iridium
Marker band lengths and locations	1 mm long, 2 mm from distal tip 3 mm long, spade-shaped at entry port
Coating	Hydrophilic, outer layer of distal 21 cm
Pushwire length	125 cm
Tapered pushwire portion	10 cm
On-ramp length	4 cm
On-ramp material	Nylon-based polymer
TruFlex™ tip	2 mm
Shelf life	2 years

DIMENSIONAL COMPARISON

French Size (F)	GEC Name	I.D. (in)	O.D. (in)	Required GC I.D. (in)
5.5	GuideLiner™* V3 GEC ⁶	0.051	0.063	6 F ≥ 0.066
6	Telescope™ GEC	0.056	0.067	6 F ≥ 0.070
6	GuideLiner™* V3 GEC ⁶	0.056	0.067	6 F ≥ 0.070
6	Guidezilla™* II GEC ⁷	0.057	0.067	6 F ≥ 0.070
7	Telescope™ GEC	0.062	0.075	7 F ≥ 0.078
7	GuideLiner™* V3 GEC ⁶	0.062	0.075	7 F ≥ 0.078
7	Guidezilla™* II GEC ⁷	0.063	0.073	7 F ≥ 0.078

Heartrail

Large I.D. & Superb Back up force

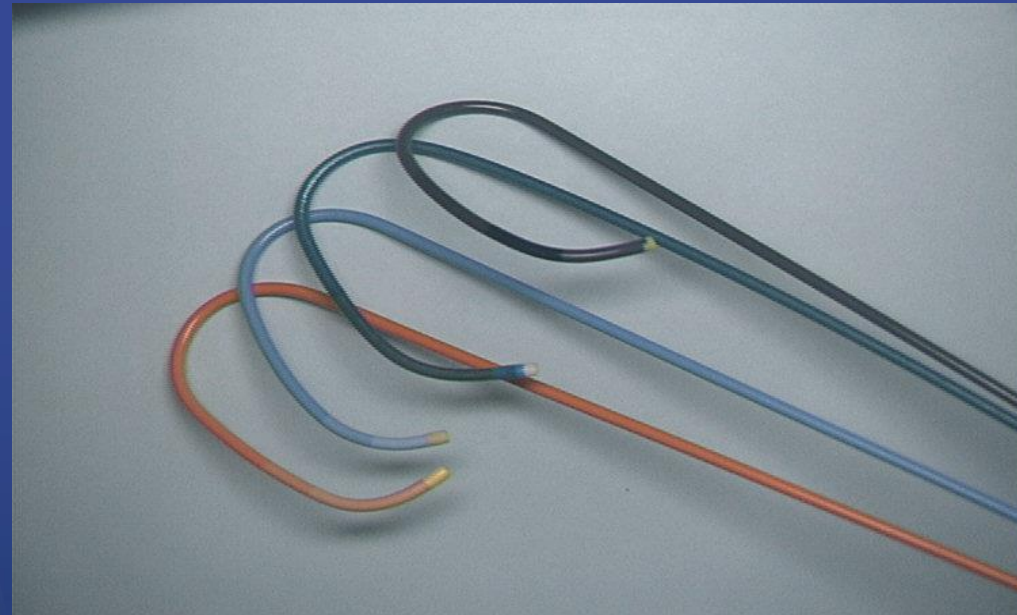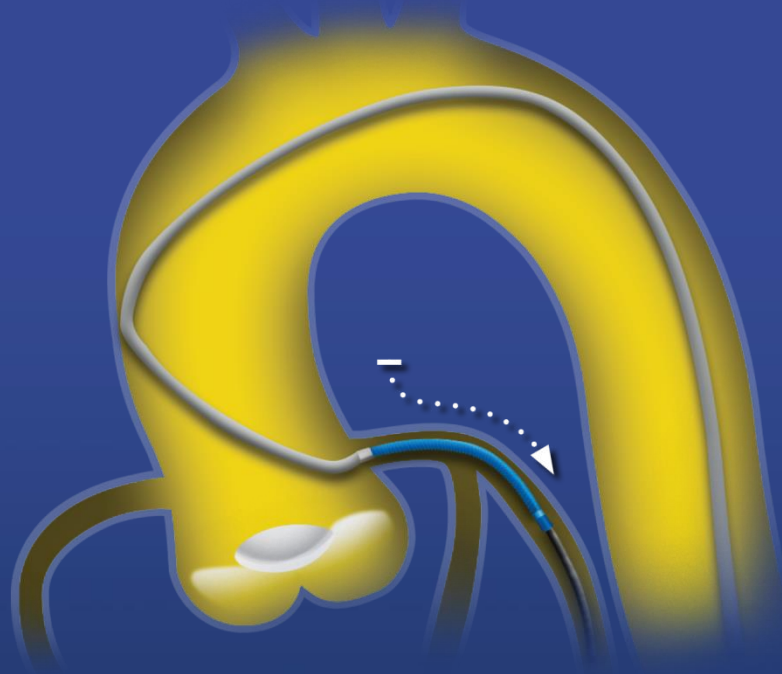

ARTIST trial

Balloon angioplasty (PTCA) vs. Rotablation in ISR (PTCR)

TABLE 4 Angiographic Outcome

	PTCA (n = 138)	PTCR (n = 139)	p Value
MLD after rotational ablation (mm)	—	1.33 ± 0.39	
Mean diameter after rotational ablation (mm)	—	1.7 ± 0.28	
Diameter stenosis after rotational ablation (%)	—	35 ± 15	
Final MLD (mm)	1.9 ± 0.3	1.9 ± 0.4	0.57
Final mean diameter (mm)	2.2 ± 0.35	2.2 ± 0.37	0.2
Final diameter stenosis (%)	29 ± 10	28 ± 12	0.38
Acute gain (mm)	1.3 ± 0.4	1.4 ± 0.4	0.45
Acute gain index	50 ± 16	52 ± 16	0.43
Final plaque area (mm ²)	6.4 ± 5.2	6.8 ± 5.4	0.55
Plaque area reduction (%)	69 ± 17	68 ± 17	0.68
Angiographic success	139/146 (95%)	144/152 (94%)	1.0
Diameter stenosis ≤30%	78/137 (57%)	87/143 (61%)	0.54


TABLE 5 Angiographic Outcome After Six Months

	PTCA (n = 123)	PTCR (n = 131)	p Value
Diameter stenosis (%)	56 ± 20	64 ± 22	0.005
MLD (mm)	1.2 ± 0.6	1.0 ± 0.6	0.008
Mean stenosis diameter (mm)	1.83 ± 0.74	1.7 ± 0.45	0.03
Late loss (mm)	0.68 ± 0.5	0.92 ± 0.6	0.0015
Loss index	50 ± 46	69 ± 42	0.0007
Net gain (mm)	0.67 ± 0.5	0.45 ± 0.6	0.0019
Net gain index	24.5 ± 20	16.8 ± 22	0.005
Neo-plaque area (mm ²)	5.1 ± 5.8	6.1 ± 6.3	0.25
Net plaque reduction (mm ²)	11.6 ± 14	7.9 ± 12	0.04
Restenosis rate (%)	51.2	64.9	0.027


COBRA study

A randomized comparison of balloon angioplasty versus rotational atherectomy in complex coronary lesions

	RA (n=252)	PTCA (n=250)	P value
Procedural success	85%	78%	0.038
6 months success	48.9%	51.1%	0.333
Major cardiac events during follow up			
Q wave MI	0.5%	0%	
CABG	4.2%	6.5%	
Death	0%	0%	

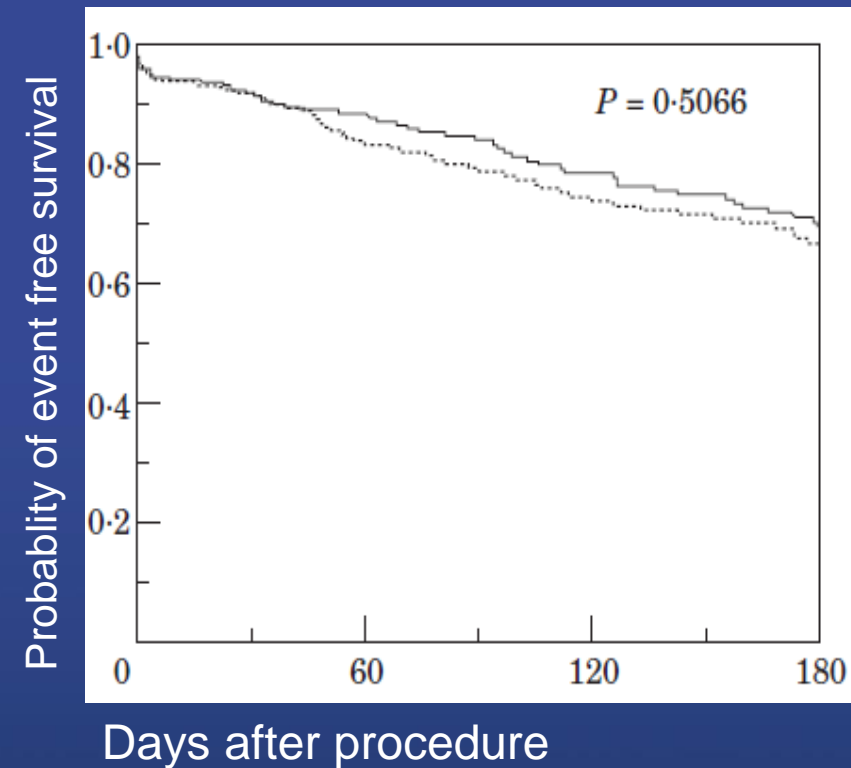

ROTAXUS; Procedural Outcomes

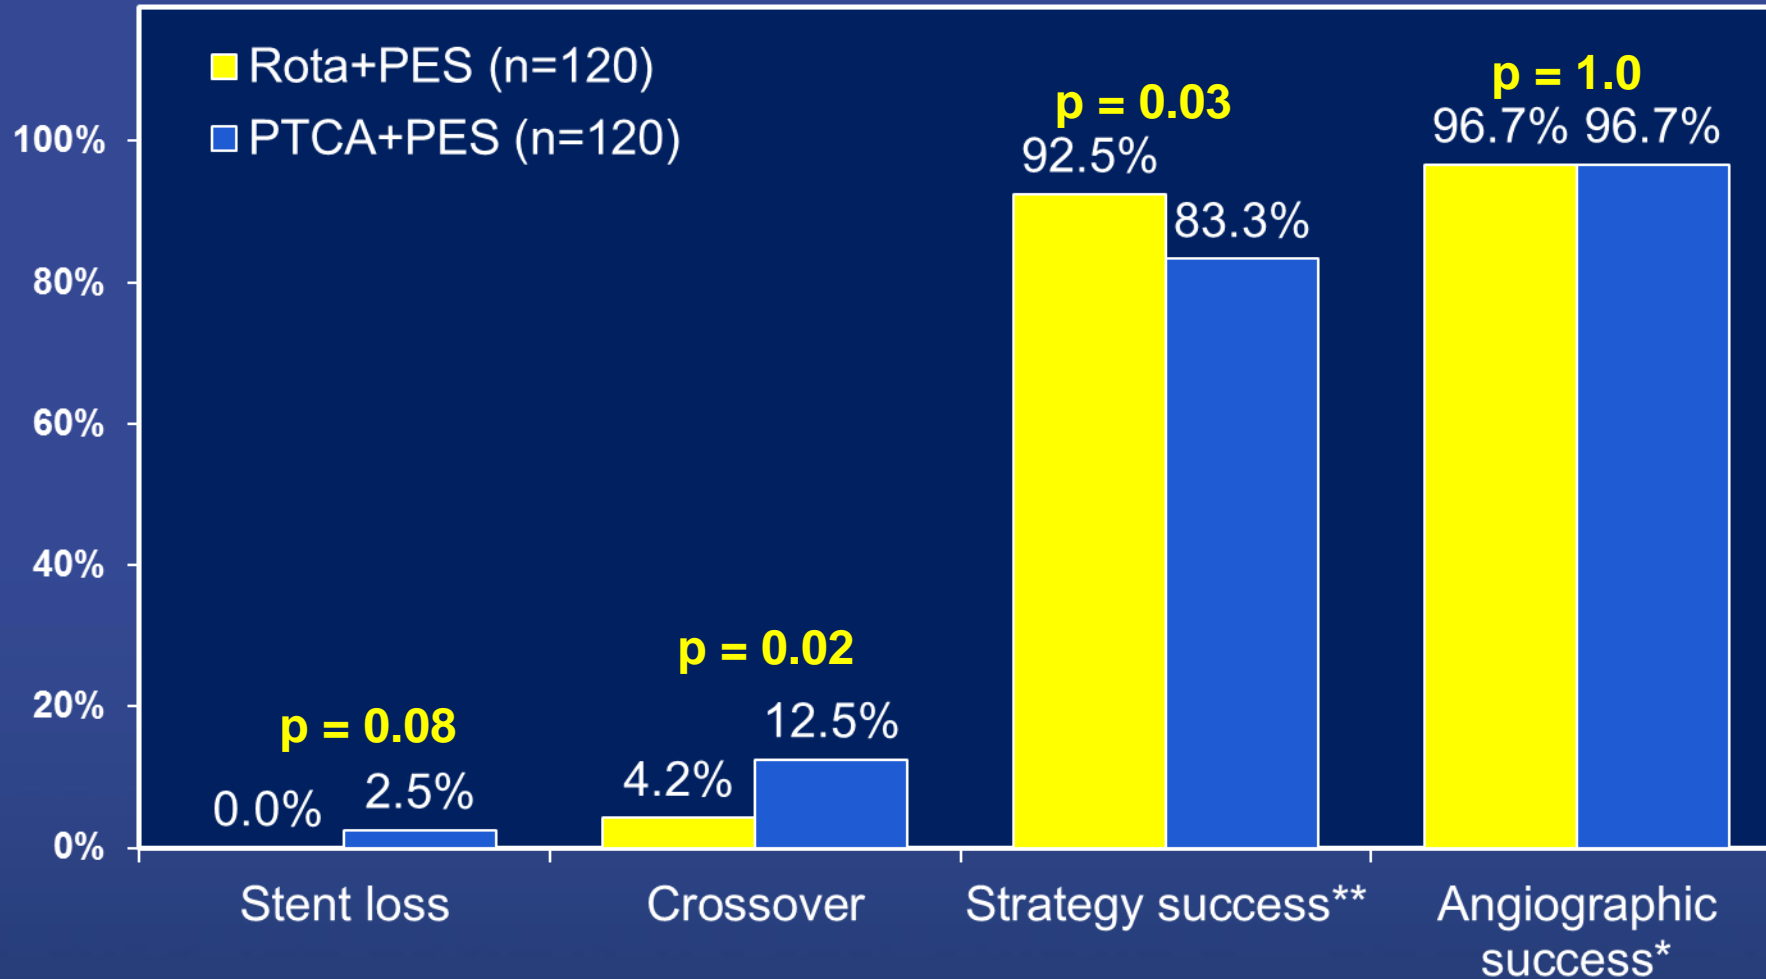


* Defined as <20% residual stenosis + TIMI 3 flow



** Defined as angiographic success with no crossover or stent loss

ROTAXUS

Strategy Success according to calcification

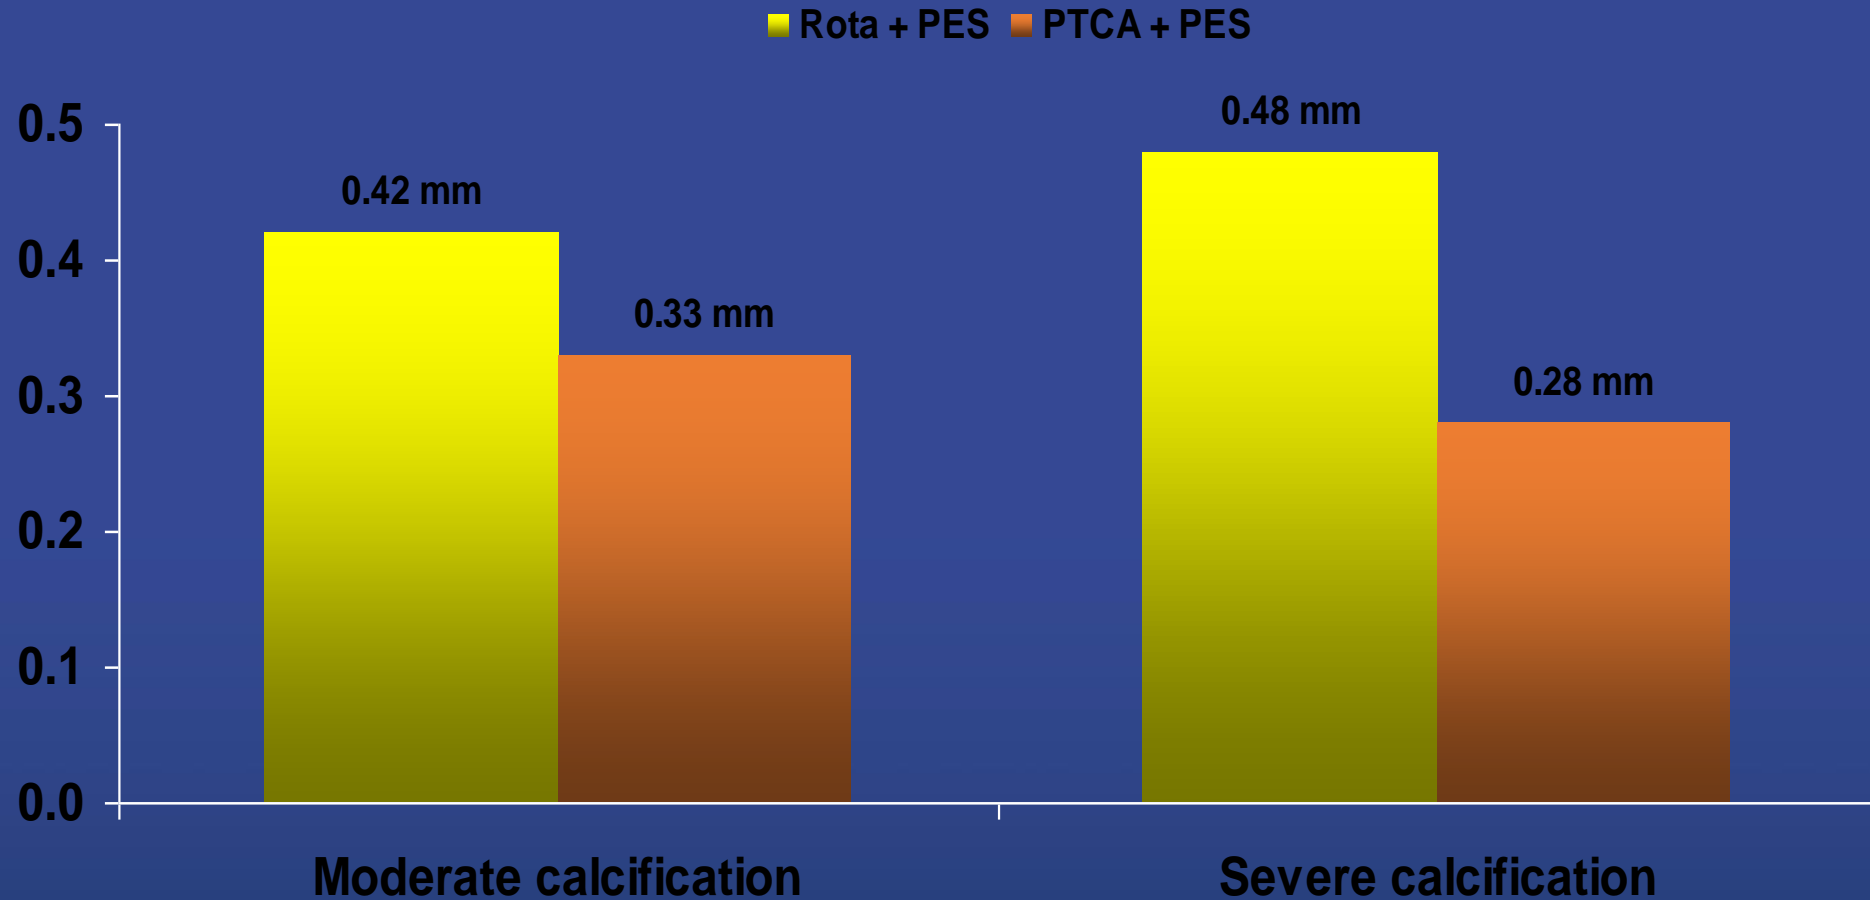

Rotaxus ; 2 year clinical outcome

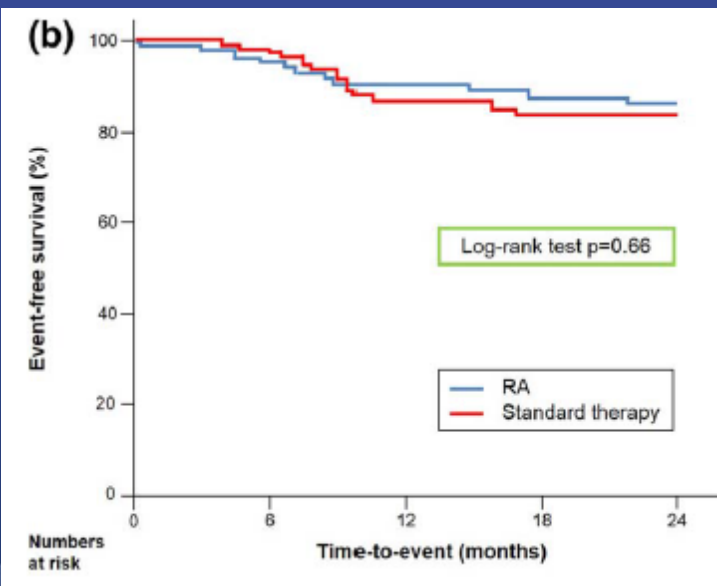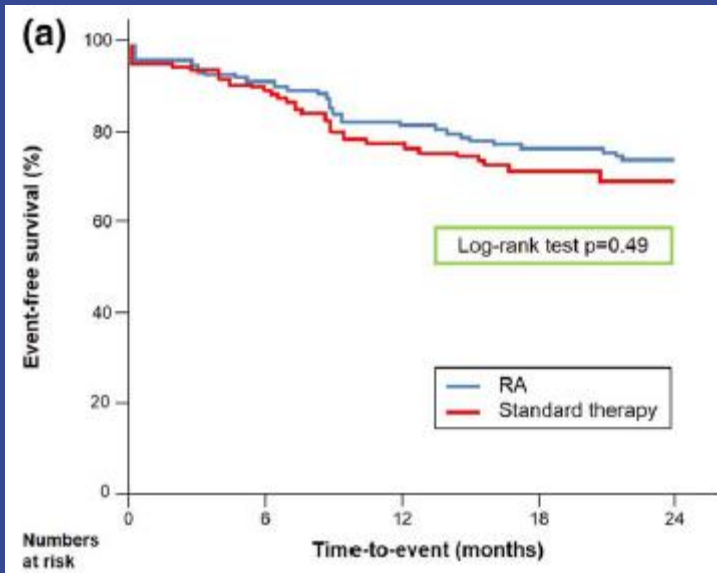

	RA+DES (n=109)	DES (n=108)	P value
Procedure success	92.5%	83.3	0.03
MACE	29.4%	34.3%	0.47
Death	8.3%	7.4%	1.00
MI	8.3%	6.5%	0.8
TLR	13.8%	16.7%	0.58
TVR	19.3%	22.2%	0.62


Increase procedure success
But does not increase clinical outcome

PREPARE-CALC Trial

Study design


Prospective, randomized, active controlled clinical trial in 2 German centers

PCI in 200 patients with severely calcified lesions

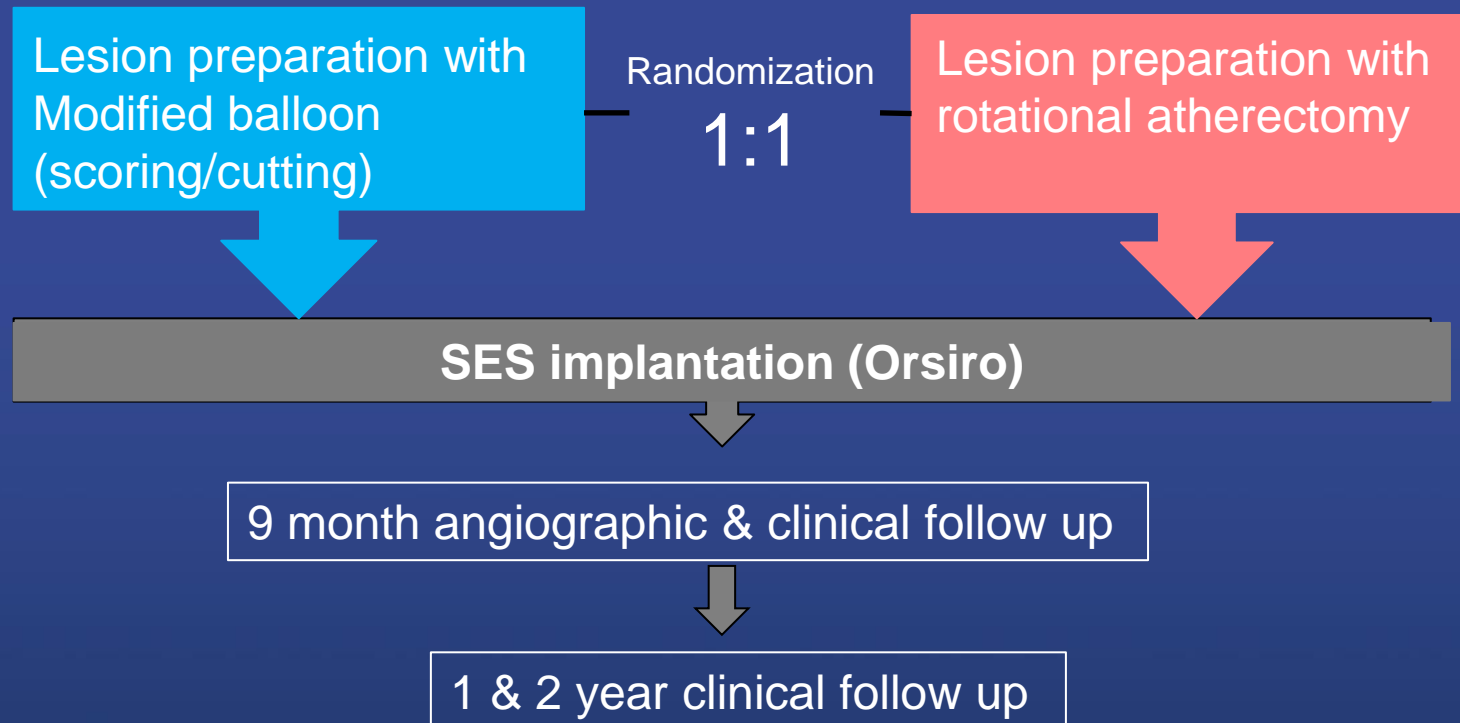

PREPARE-CALC Trial

Co-Primary Endpoint – In stent LLL at 9 Month

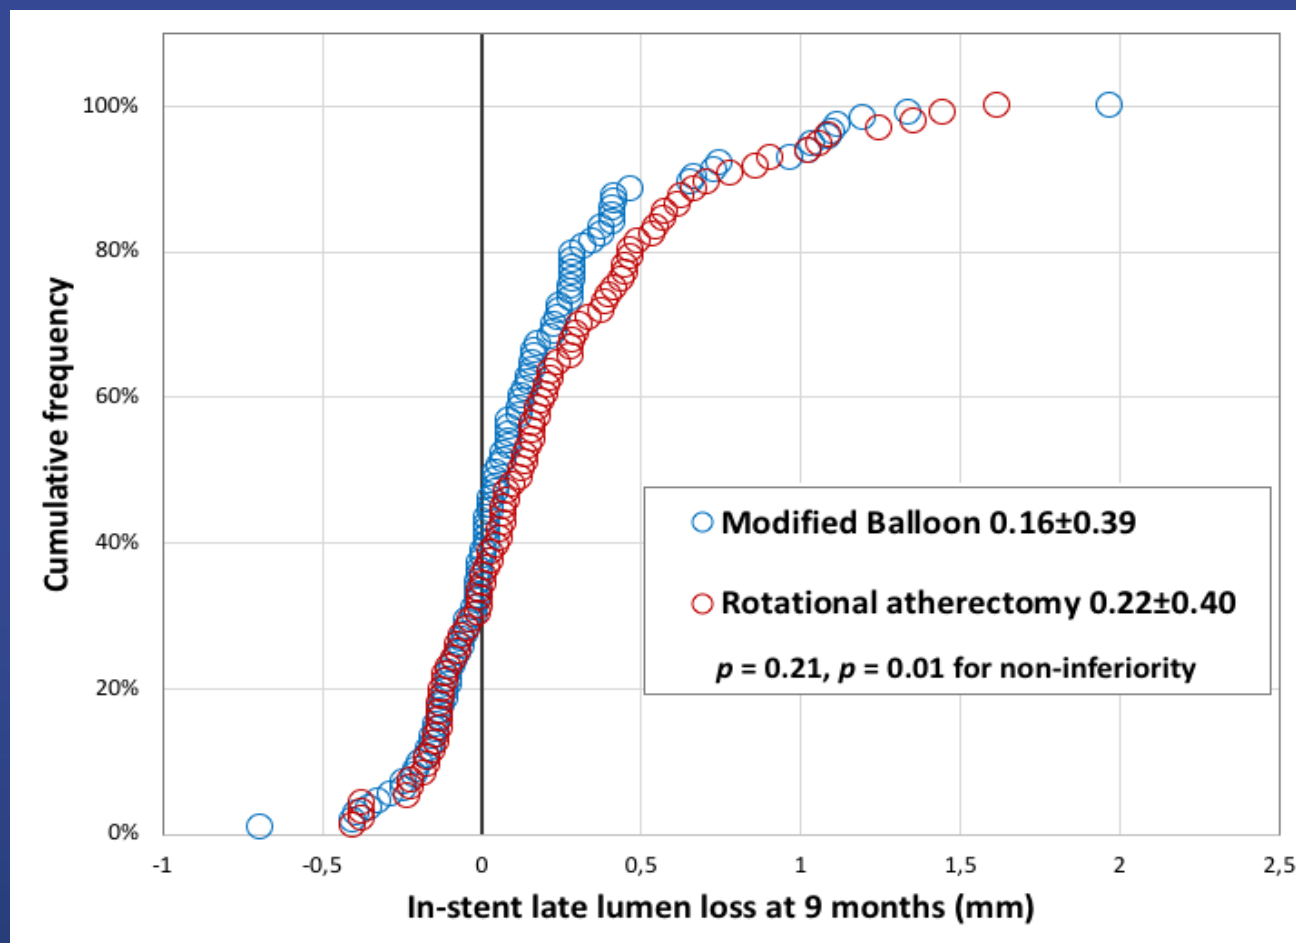

PREPARE-CALC Trial

QCA 9 months


	Modified balloon (n = 112 lesions)	Rotational atherectomy (n = 97 lesions)	p-value
Minimal lumen diameter (mm)			
In-stent	2.68±0.59	2.64±0.51	0.59
In-segment	2.50±0.54	2.50±0.55	0.96
Diameter stenosis (%)			
In-stent	18.83±13.42	19.75±11.54	0.49
In-segment	22.40±11.36	23.30±11.43	0.52
Late lumen loss (mm)			
In-stent	0.16±0.40	0.22±0.41	0.21
In-segment	0.07±0.52	0.18±0.74	0.25
Binary restenosis (%)			
In-stent	6 (5.3%)	2 (2.1%)	0.30
In-segment	5 (4.5%)	2 (2.1%)	0.32

PREPARE-CALC Trial

Clinical outcome 9 months

	Modified balloon (n = 100 pts.)	Rotational atherectomy (n = 100 pts.)	p-value
Death	2 (2%)	2 (2%)	1.00
Cardiac death	1 (1%)	1 (1%)	1.00
Non-cardiac death	1 (1%)	1 (1%)	1.00
Myocardial infarction	3 (3%)	2 (2%)	1.00
Target vessel MI	1 (1%)	2 (2%)	1.00
Periprocedural MI	1 (1%)	2 (2%)	1.00
Spontaneous MI	2 (2%)	0 (0%)	0.50
Stent thrombosis (def./prob.)	0 (0%)	0 (0%)	1.00
TVR	8 (8%)	3 (3%)	0.21
Target vessel failure	8 (8%)	6 (6%)	0.78

PREPARE-CALC Trial Clinical outcome 2-year

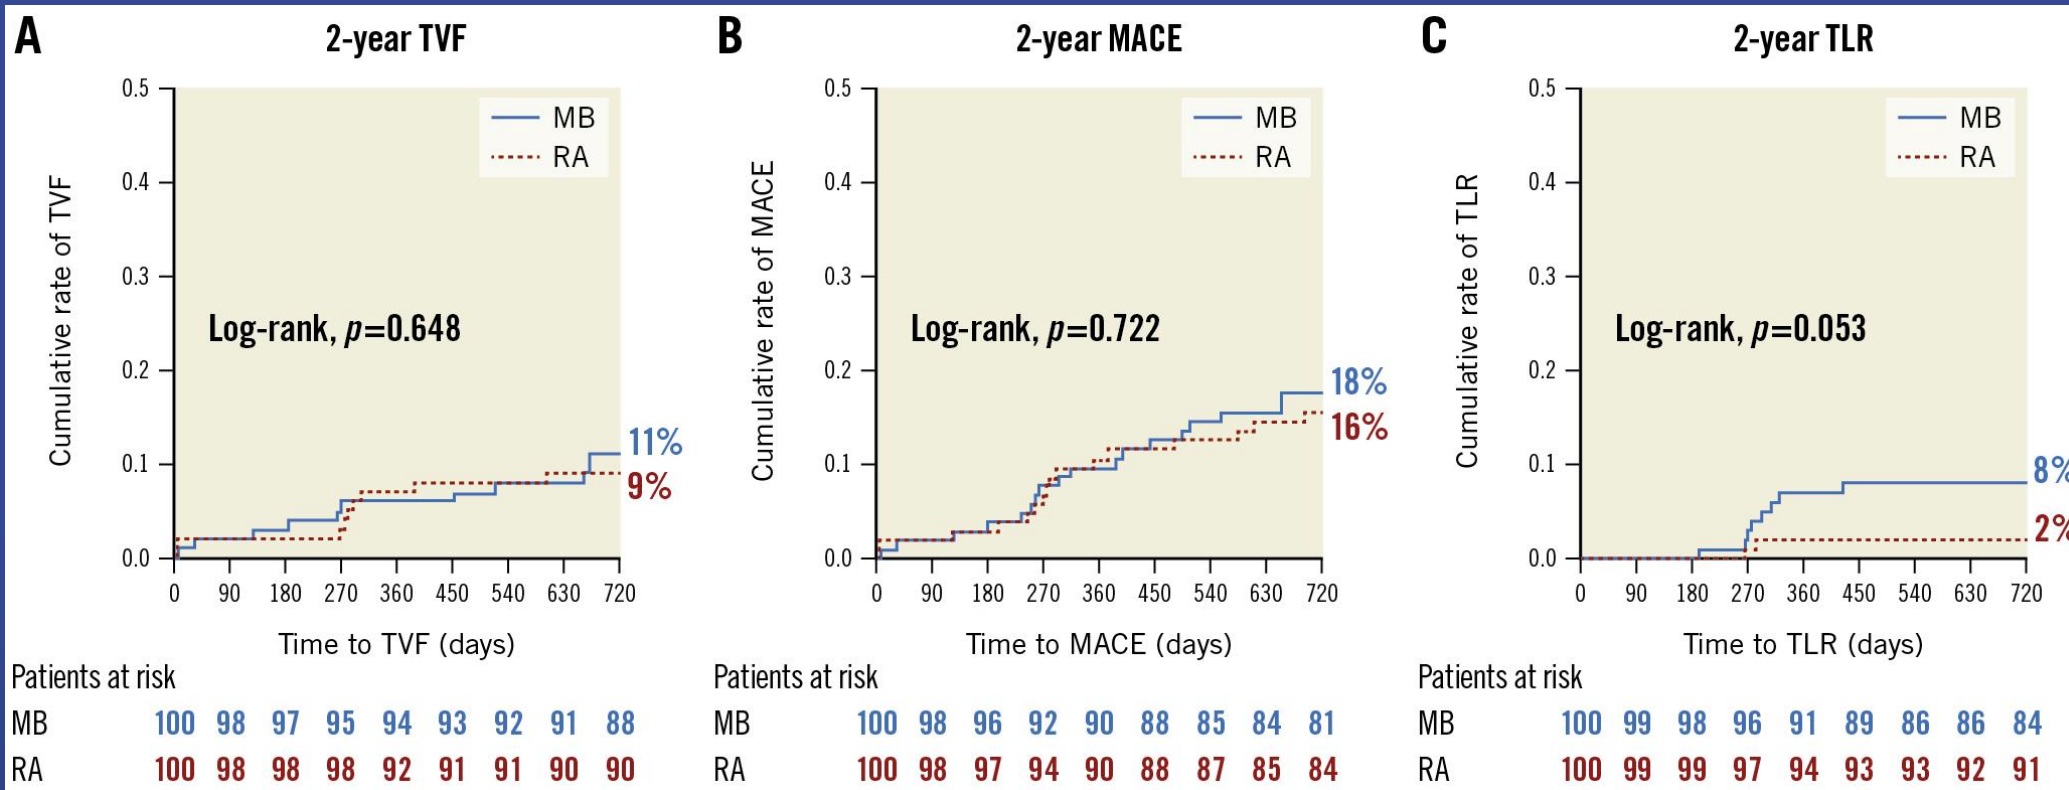



PREPARE-CALC-COMBO Study

Combined rotational atherectomy and cutting balloon angioplasty prior to drug-eluting stent implantation in severely calcified coronary lesions

- **To assess whether the Rota-Cut combination improves stent performance in severely calcified coronary lesions**
- **Prospective, single-arm, single center study**
- **Primary endpoint : in-stent acute lumen gain(ALG), stent expansion(SE)**


PREPARE-CALC-COMBO Study

Combined rotational atherectomy and cutting balloon angioplasty prior to drug-eluting stent implantation in severely calcified coronary lesions

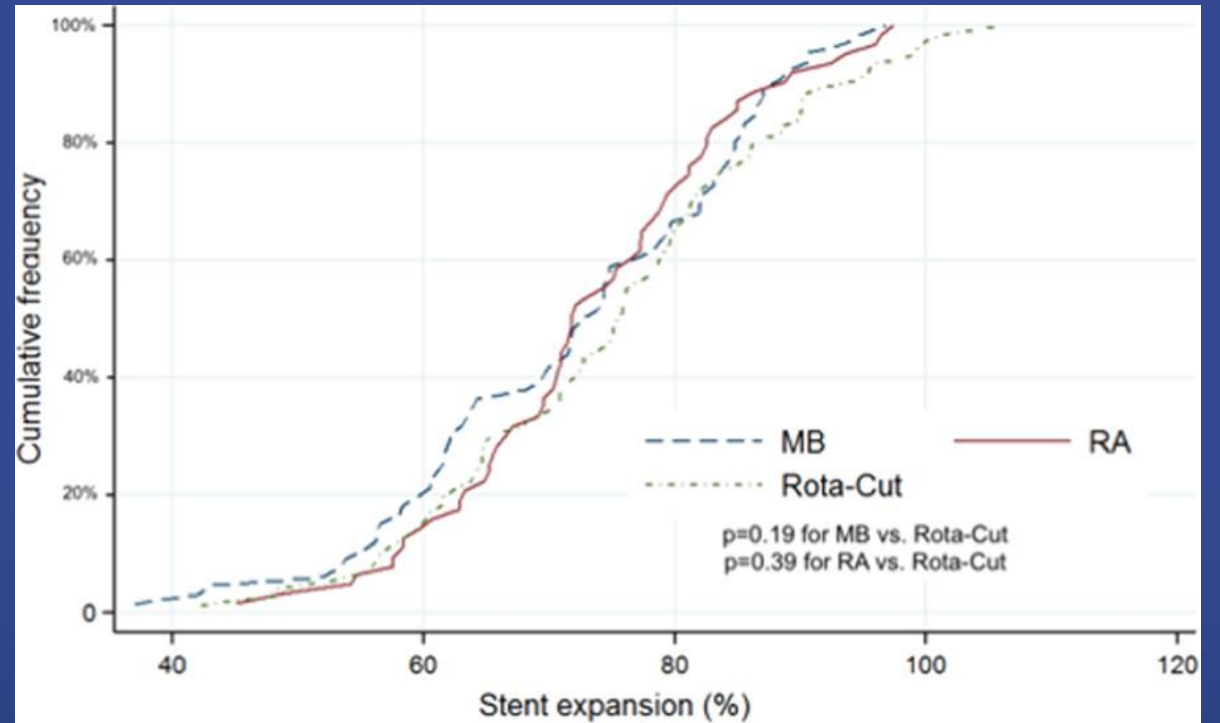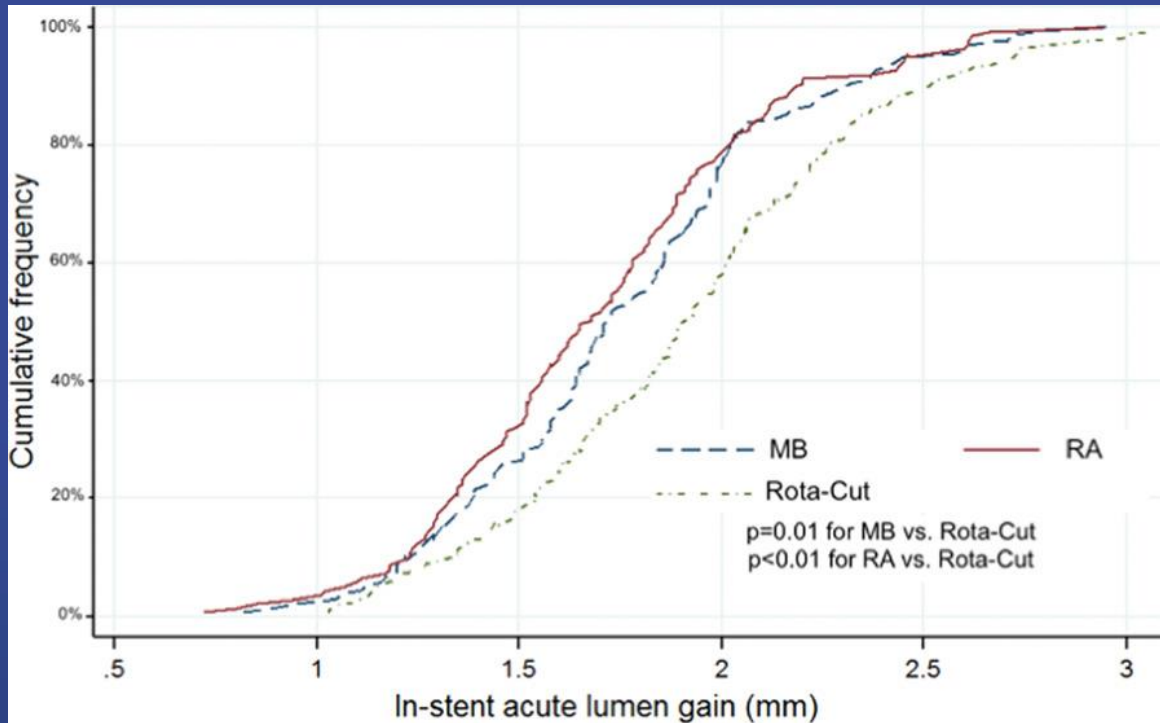


DIRO Study

- Direct Comparison of Rotational vs Orbital Atherectomy for Calcified Lesions Guided by Optical Coherence Tomography

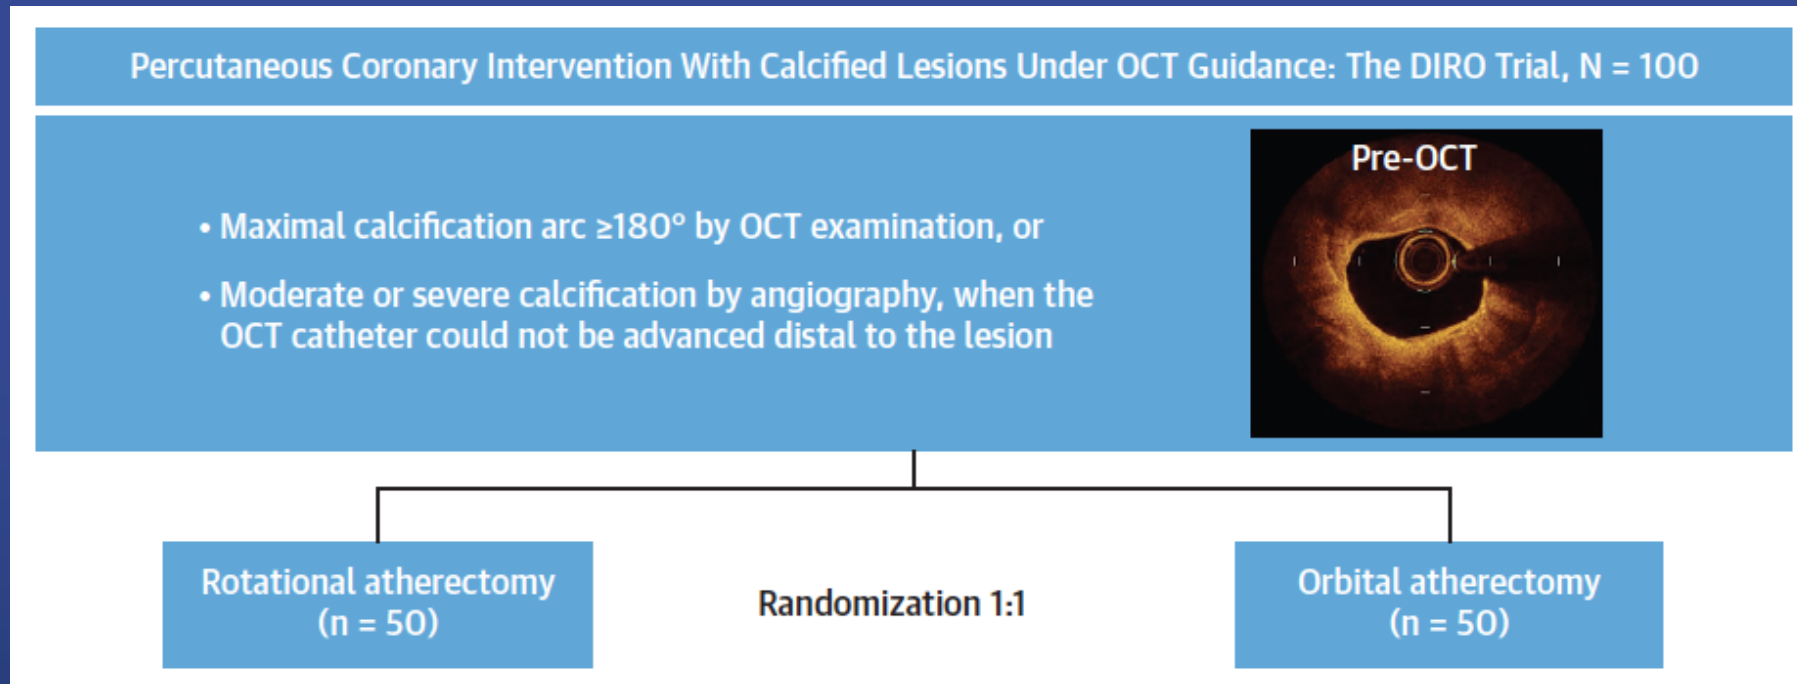

Okamoto N, et al. J Am Coll Cardiol Interv. 2023;16(17):2125–2136.

DIRO Study

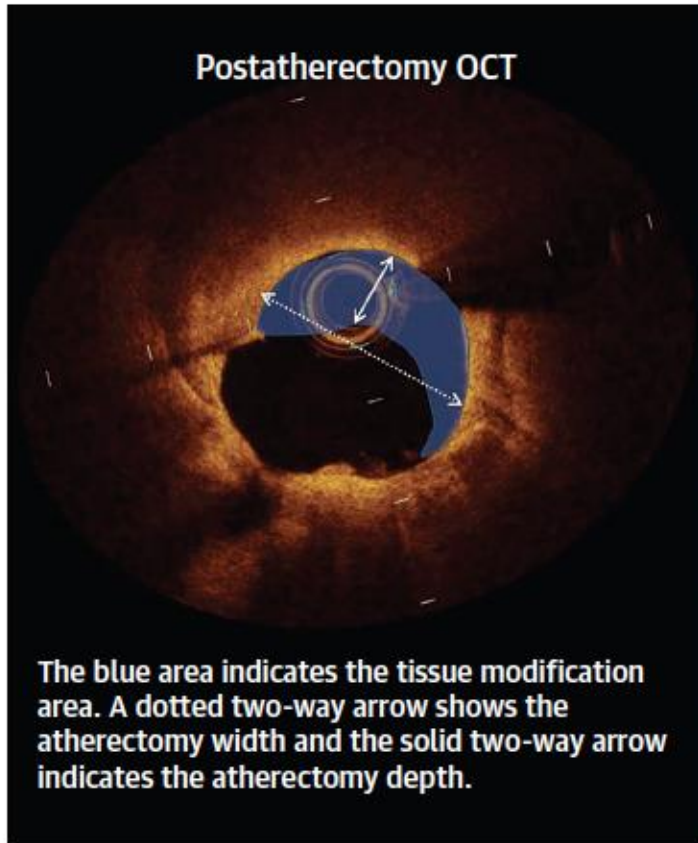

	RA	OA	P Value
Maximum tissue modification area, mm ²	1.24 (0.84-1.74)	0.89 (0.59-1.11)	<0.01
Atherectomy width, mm	1.50 (1.32-1.89)	1.22 (1.12-1.40)	<0.01
Atherectomy depth, mm	0.54 (0.39-0.83)	0.55 (0.31-0.73)	0.62
Percentage of lumen area increase, %	72.2 (49.0-98.3)	39.2 (17.0-48.1)	<0.01
Ratio of atherectomy width to burr size	0.94 (0.79-0.98)	0.98 (0.89-1.12)	0.03
Stent expansion assessed by distal reference, %	99.5 (89.3-107.3)	90.6 (80.0-102.3)	0.02
Stent expansion assessed by mean reference, %	72.2 (60.6-86.3)	64.1 (54.0-77.7)	0.05

- Procedural outcomes including periprocedural MI were comparable
- Clinical outcomes at 8 months were similar



ECLIPSE

Evaluation of Treatment Strategies for Severe **Ca**lcif**i**c Coronary Arteries: Orbital Atherectomy vs. Conventional Angioplasty **P**rior to Implantation of Drug Eluting **S**tEnts

~2000 pts with severely calcified lesions; ~150 US sites

Randomize

1:1

Orbital Atherectomy Strategy

(1.25 mm Classic Crown followed by balloon pre-dilation)

2nd generation DES implantation and optimization

Conventional Angioplasty Strategy

(Conventional and/or specialty balloons per operator discretion)

2nd generation DES implantation and optimization


1° endpoints: 1) Post-PCI in-stent MSA by OCT (N~500 in imaging sub-study)
2) 1-year TVF (all subjects)

2° endpoints: 1) Procedural Success (Stent deployed w/RS<20% & no maj complications)
2) Strategy Success (Procedural success w/out crossover)


ECLIPSE

Evaluation of Treatment Strategies for Severe Calcific Coronary Arteries: Orbital Atherectomy vs. Conventional Angioplasty Prior to Implantation of Drug Eluting StEnts

Primary Imaging Endpoint (OCT Cohort) Minimal stent area at maximum calcium site

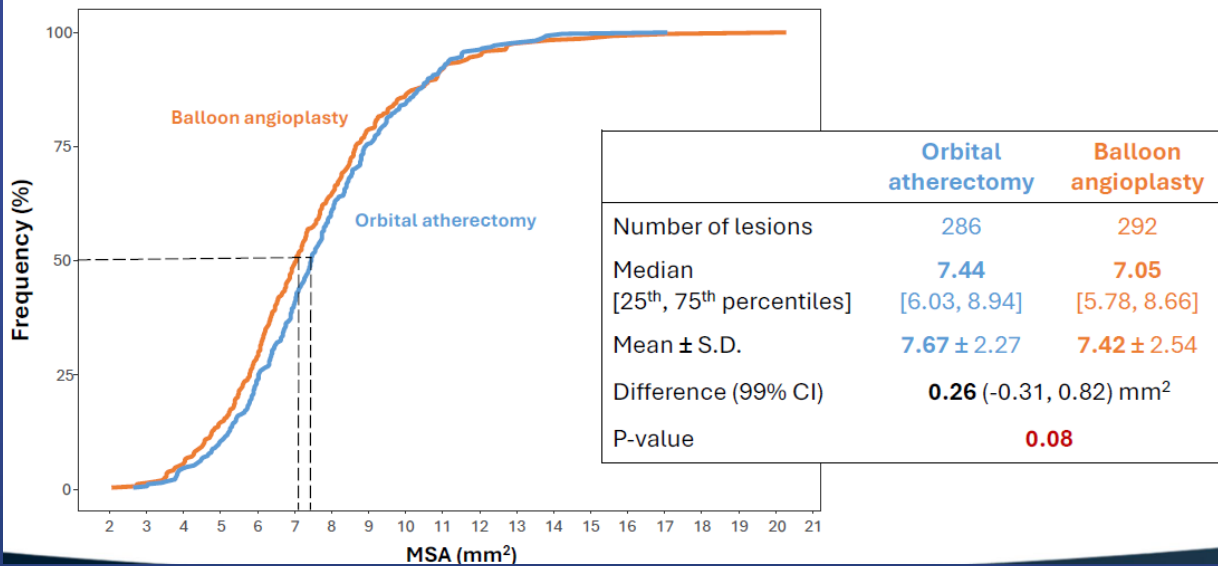

Primary Clinical Endpoint Target Vessel Failure at 1 Year

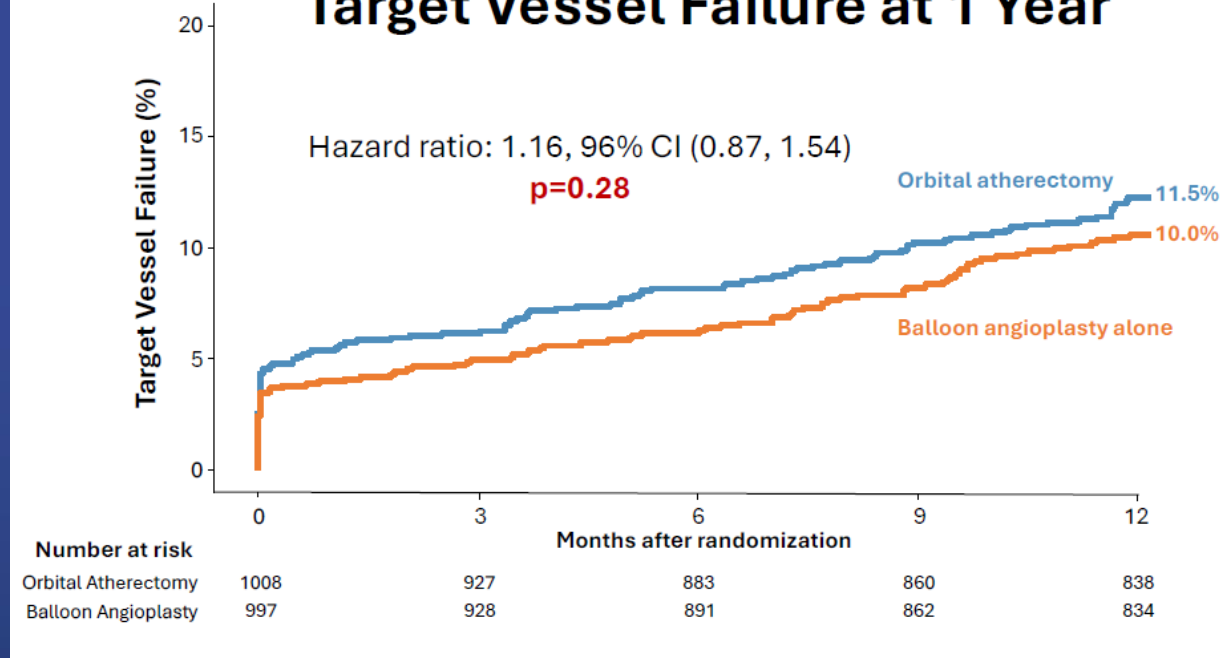



Disrupt CAD III

Intravascular Lithotripsy for Treatment of Severely Calcified Coronary Artery Disease

- **To assess safety and effectiveness of IVL in severely calcified de novo coronary lesions**
- **Prospective, single-arm multicenter study**
- **Primary safety endpoint : freedom from major adverse cardiovascular events (cardiac death, MI, or target vessel revascularization) at 30 days**
- **Primary effectiveness endpoint : procedural success**



Disrupt CAD III

Intravascular Lithotripsy for Treatment of Severely Calcified Coronary Artery Disease

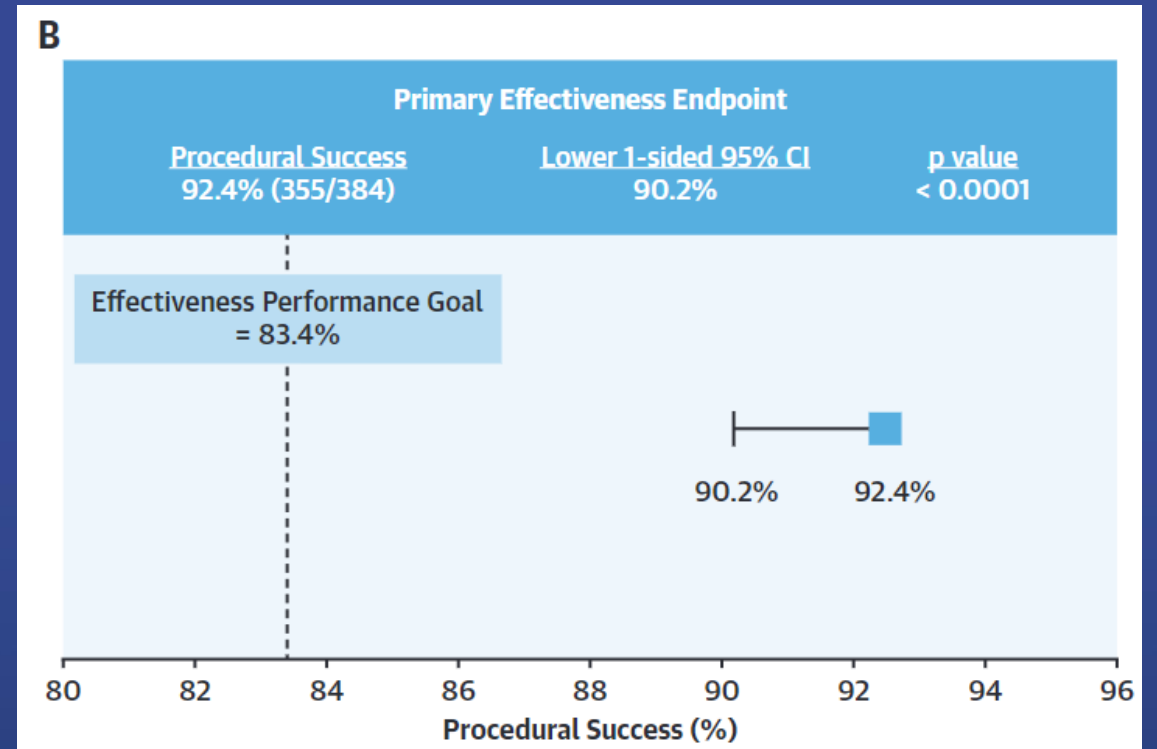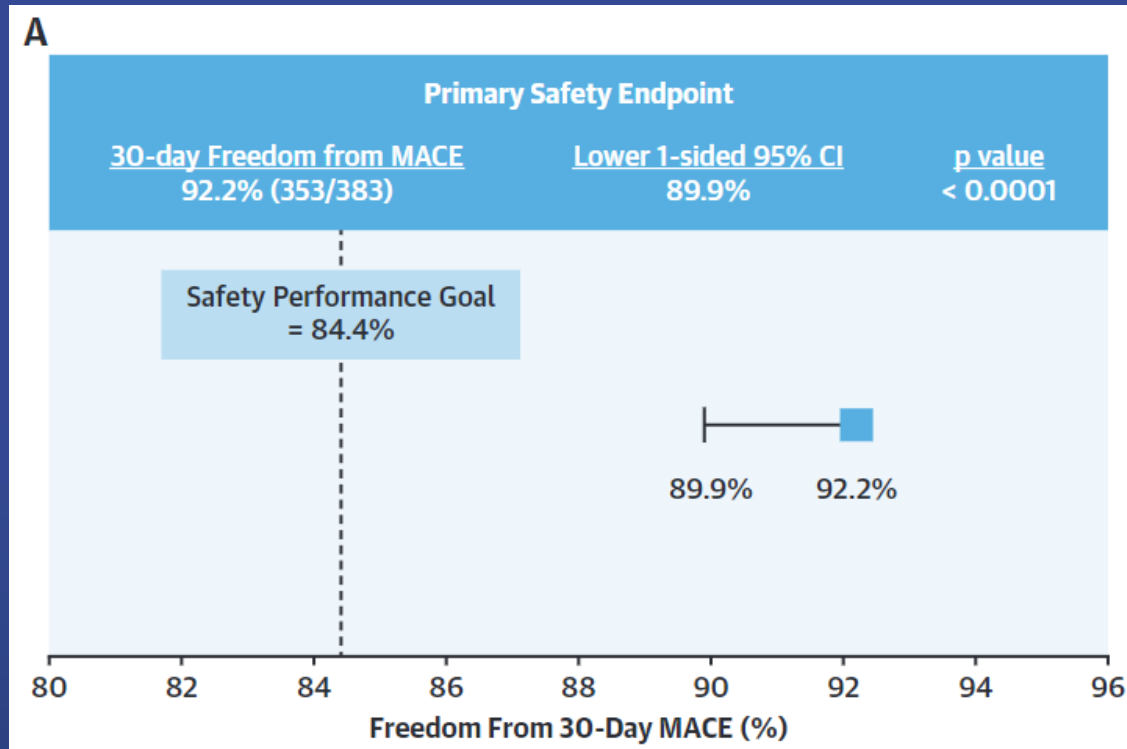

Disrupt CAD III

Intravascular Lithotripsy for Treatment of Severely Calcified Coronary Artery Disease

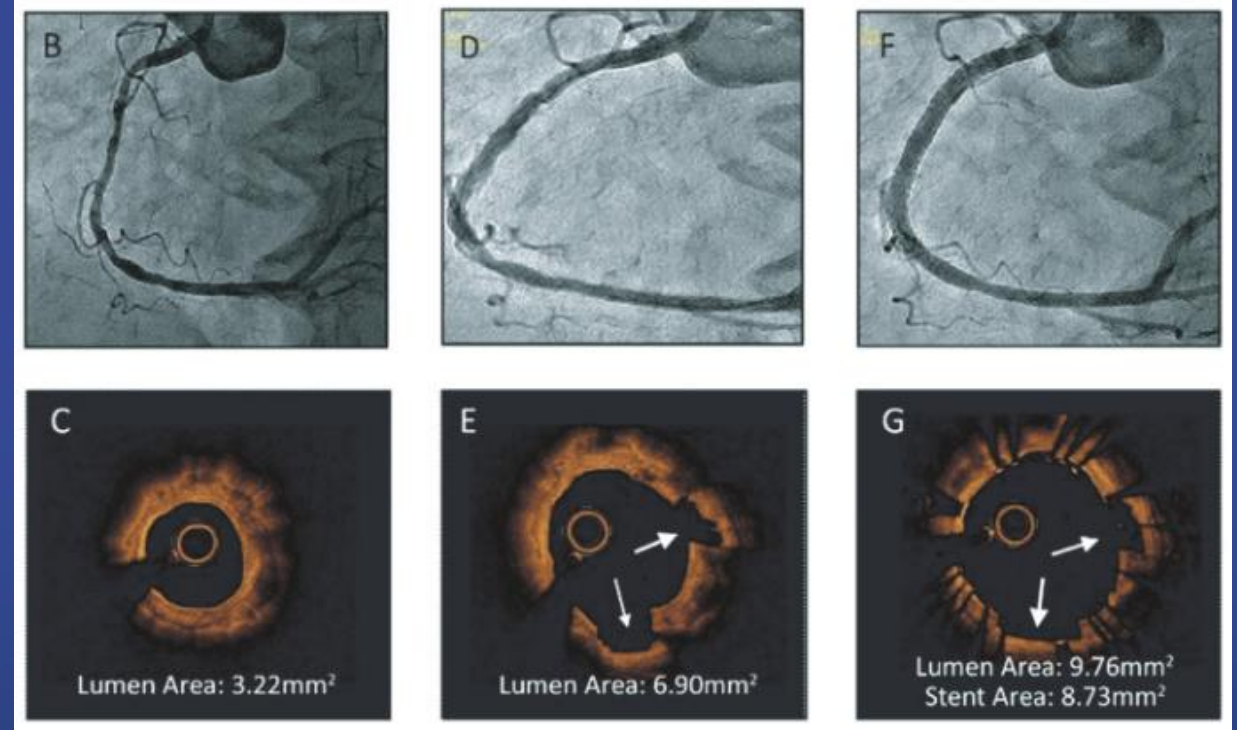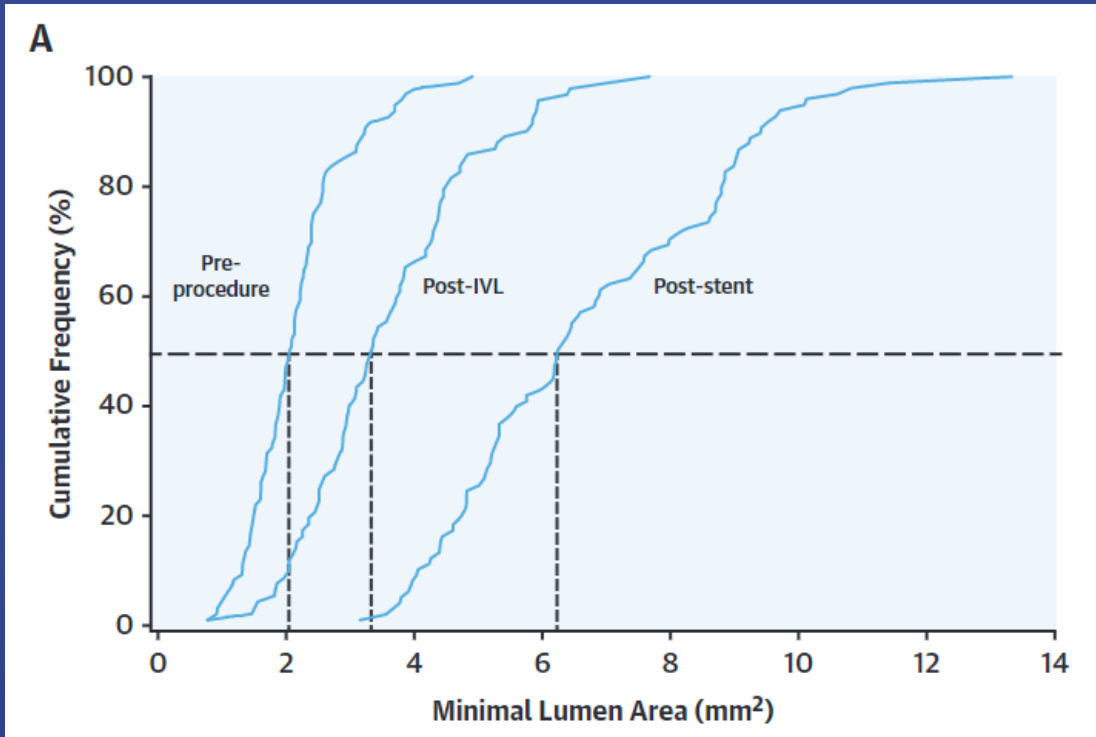

DISRUPT-CAD Studies

	DISRUPT-CAD I	DISRUPT-CAD II	DISRUPT-CAD III	DISRUPT-CAD IV	Pooled result
Patients	60	120	384	64	628
Procedural success	95%	94%	92.4%	93.8%	92.4%
Stent delivery	100%	100%	99.2%	100%	99.5%
Severe dissection	0%	0%	0.3%	0%	0.2%
Perforation	0%	0%	0.3%	0%	0.2%
Abrupt closure	0%	0%	0.3%	0%	0.2%
Slow/no flow	0%	0%	0%	0%	0%

Kereiakes, D.J. et al. J Am Coll Cardiol Intv. 2021; 14 (12) 1337–1348.

ISAR-CALC 2 trial

Randomized Comparison of Strategies to Prepare Severely Calcified Coronary Lesions 2

- **To compare a lesion preparation strategy with either super high-pressure balloon or intravascular lithotripsy in severely calcified undilatable coronary lesion**
- **Prospective, randomized, multicenter, assessors-blind, open-label study**
- **Primary end point : final angiographic minimal lumen diameter after stent implantation**

ISAR-CALC 2 trial

Randomized Comparison of Strategies to Prepare Severely Calcified Coronary Lesions 2

